


Pulsed Frequency™



MR72 Software Download, Installation and User Guide

Contents


Healthcare Professional Account Registration	3
Outside USA Account Registration.....	6
Create an Account.....	9
Download the Software	11
Chrome.....	12
Firefox	13
Internet Explorer	15
Install the Software.....	17
Connect MR72 to Your Computer.....	25
Run the Software for the First Time	27
Compiler.....	30
Main Menu.....	34
View Frequency Files in Device.....	36
Magnetic Frequency File Bank.....	38
Create Magnetic Frequency File	42
Edit Magnetic Frequency File.....	45
Create Play Magnetic Frequency File.....	48
File Storage	57
Troubleshooting.....	63
MR72 Manual Detection.....	66

Healthcare Professional Account Registration

To download the professional version of the Pulsed Frequency software, please go to www.pulsedfrequency.com. If you are a healthcare professional in the USA, click where the arrow is pointing below.




When you click the arrow, the following screen appears.

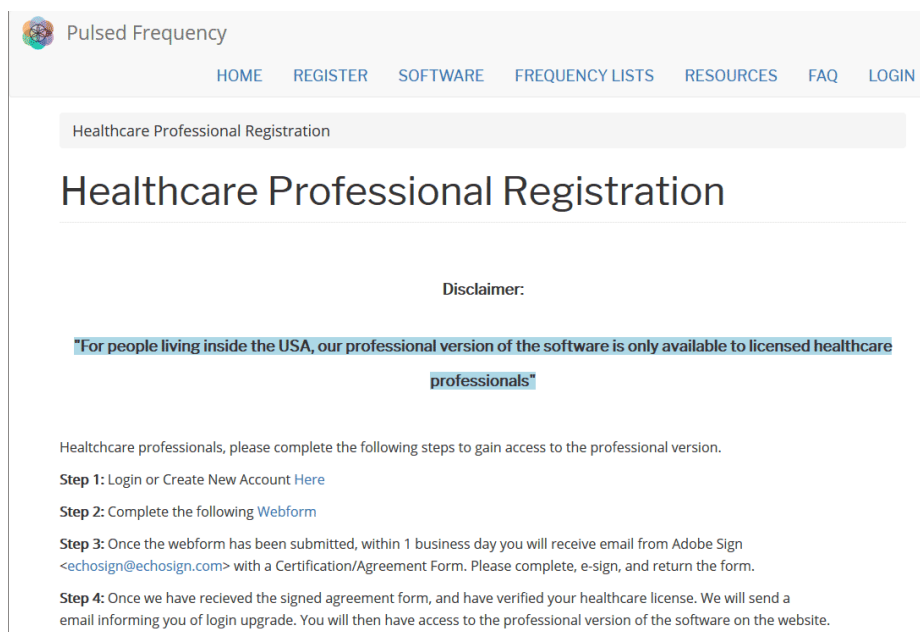


There are four steps you must follow in order to download the professional version of the software.

Step 1) Login to your account. If you don't have one, go to the **Create an Account** section of the manual.

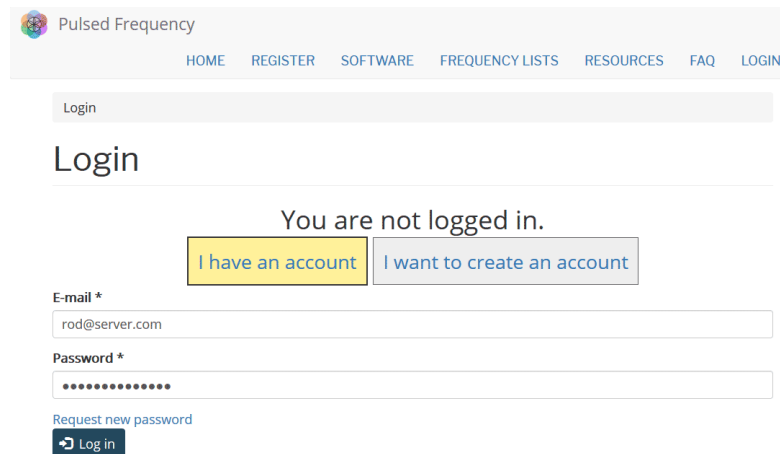


The screenshot shows the Pulsed Frequency website's login page. At the top is a navigation bar with links: HOME, REGISTER, SOFTWARE, FREQUENCY LISTS, RESOURCES, FAQ, and LOGIN. Below the navigation bar is a 'Login' section. It features a message 'You are not logged in.' with two buttons: 'I have an account' (highlighted in yellow) and 'I want to create an account'. Below these are input fields for 'E-mail *' (containing 'rod@server.com') and 'Password *' (masked with dots). There is a link for 'Request new password' and a 'Log in' button.

If you have an account, click **I have an account**. Enter your email address and password and click **Log in**.

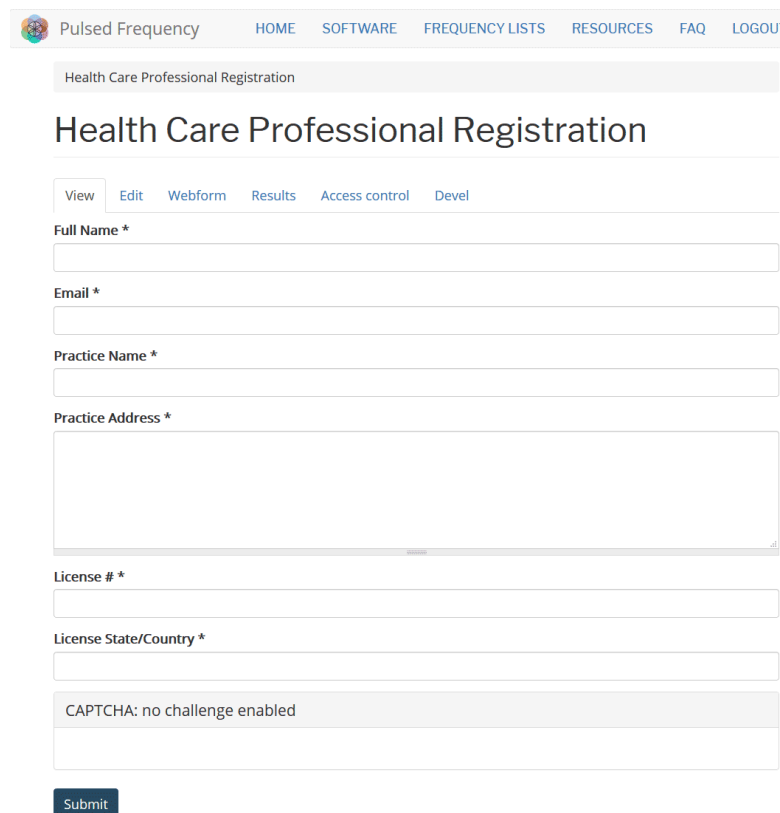

The screenshot shows the 'Health Care Professional Registration' form on the Pulsed Frequency website. The navigation bar at the top includes links: HOME, SOFTWARE, FREQUENCY LISTS, RESOURCES, FAQ, and LOGOUT. The form title is 'Health Care Professional Registration'. Below the title are tabs: View, Edit, Webform, Results, Access control, and Devel. The form contains several input fields: 'Full Name *', 'Email *', 'Practice Name *', 'Practice Address *' (a larger text area), 'License # *', and 'License State/Country *'. At the bottom of the form is a 'CAPTCHA: no challenge enabled' section and a 'Submit' button.

Step 2) Fill out form that is displayed, then click the **Submit** button.

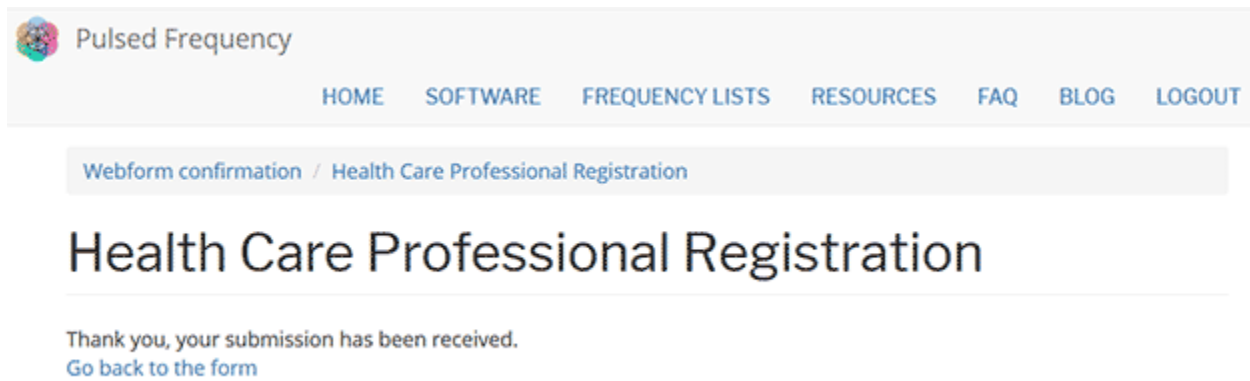

This page is displayed once you have submitted your form.

Step 3) Wait for 1-2 business days. At the end of that time, you will receive an email from Adobe Sign (echosign@echosign.com) with a Certification/Agreement Form. Please complete the form, e-sign, and return the form.

Step 4) Once your signed agreement form has been received and your healthcare license has been verified, you will receive an email notifying you that your login has been upgraded to a healthcare professional login.


When you receive this email, login to your account and you will be able to download the professional version of the software.

Outside USA Account Registration

To download the professional version of the Pulsed Frequency software, please go to www.pulsedfrequency.com. If you live outside the USA, click where the arrow is pointing below.




When you click the arrow, the following screen appears.

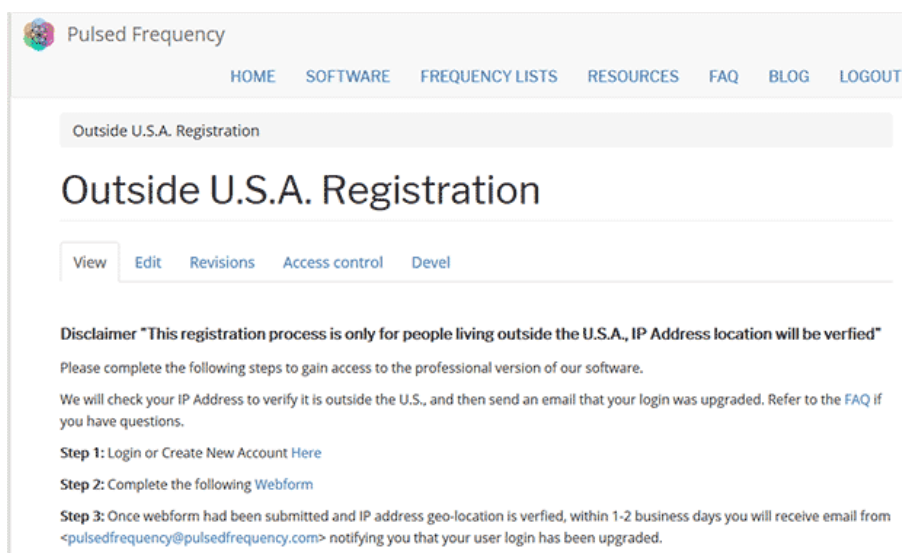


There are three steps you must follow in order to download the professional version of the software.

Step 1) Login to your account. If you don't have one, go to the **Create an Account** section of the manual.

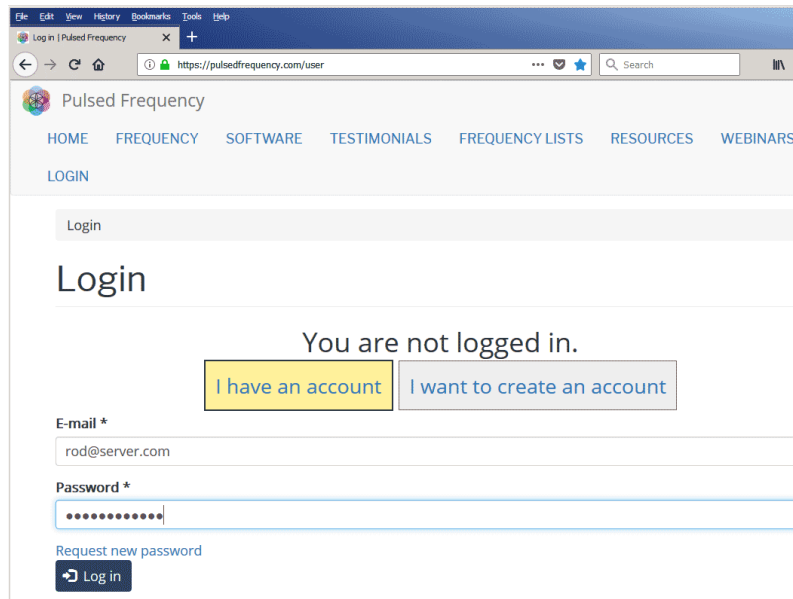


The screenshot shows a web browser window with the URL <https://pulsedfrequency.com/user>. The page title is "Pulsed Frequency" and the navigation menu includes HOME, FREQUENCY, SOFTWARE, TESTIMONIALS, FREQUENCY LISTS, RESOURCES, and WEBINARS. Below the navigation menu is a "LOGIN" section. The login form has a heading "Login" and a message "You are not logged in." Below this message are two buttons: "I have an account" (highlighted in yellow) and "I want to create an account". The form includes fields for "E-mail *" (containing "rod@server.com") and "Password *" (containing "*****"). There is a link "Request new password" and a "Log in" button.

If you have an account, click **I have an account**. Enter your email address and password and click **Log in**.

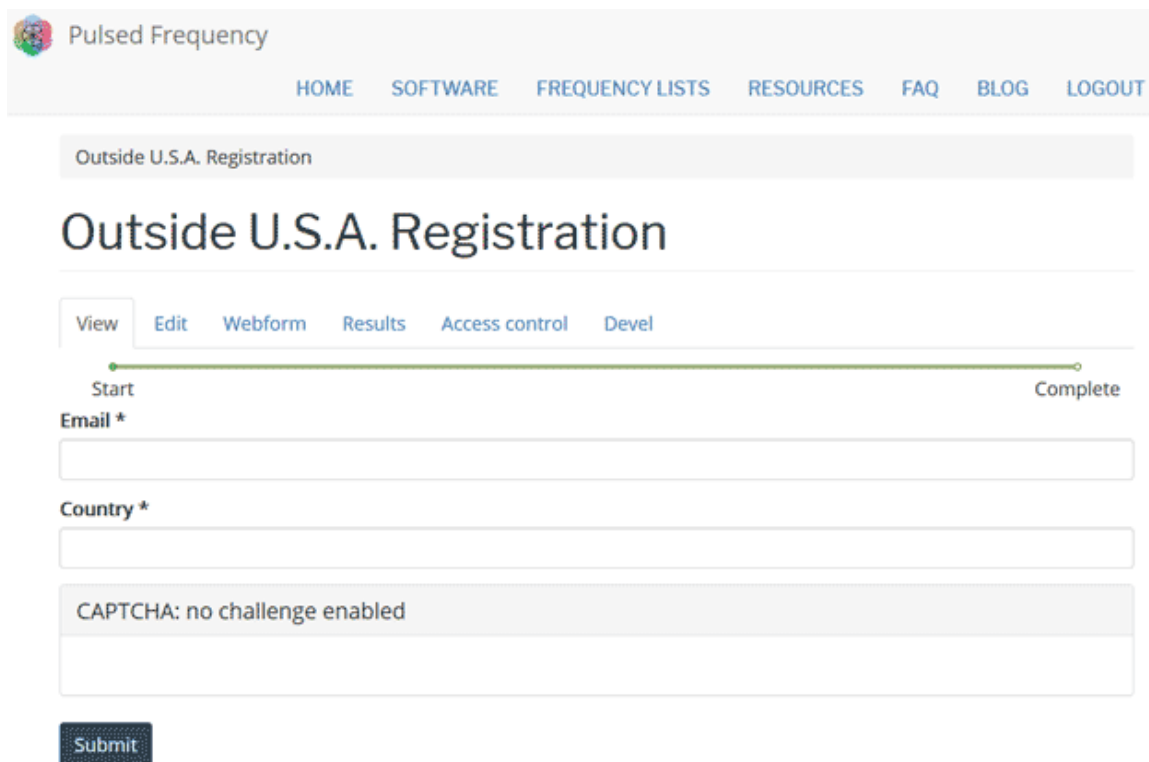

The screenshot shows the "Outside U.S.A. Registration" form on the Pulsed Frequency website. The navigation menu includes HOME, SOFTWARE, FREQUENCY LISTS, RESOURCES, FAQ, BLOG, and LOGOUT. The form has a heading "Outside U.S.A. Registration" and a progress bar with "Start" and "Complete" markers. Below the progress bar are tabs: View, Edit, Webform, Results, Access control, and Devel. The form includes fields for "Email *" and "Country *". Below these fields is a CAPTCHA section with the text "CAPTCHA: no challenge enabled". At the bottom of the form is a "Submit" button.

Step 2) Fill out form that is displayed, then click the **Submit** button.

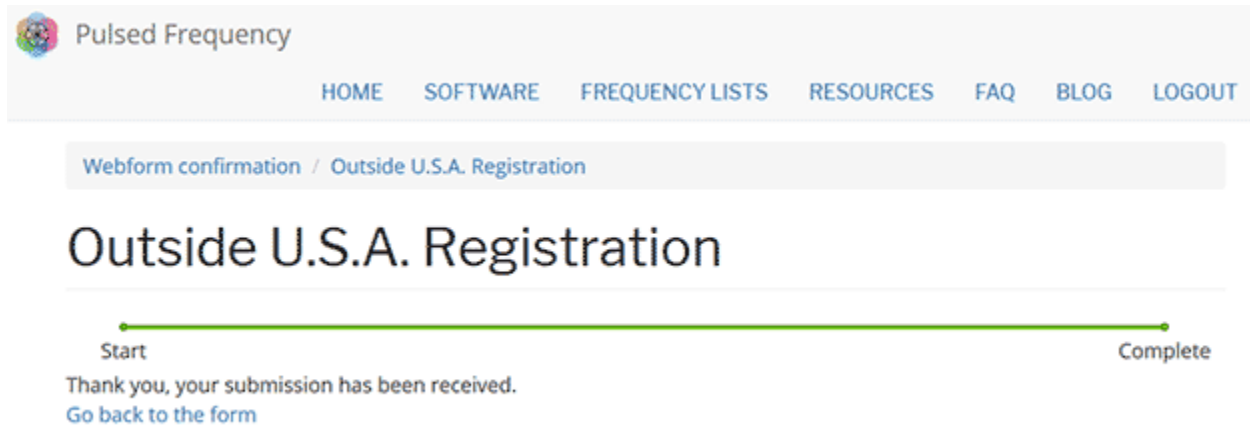

The screenshot shows the Pulsed Frequency website header with a logo and navigation links: HOME, SOFTWARE, FREQUENCY LISTS, RESOURCES, FAQ, BLOG, and LOGOUT. Below the header is a breadcrumb trail: Webform confirmation / Outside U.S.A. Registration. The main heading is 'Outside U.S.A. Registration'. A progress bar is shown with a green line from 'Start' to 'Complete'. Below the bar, it says 'Thank you, your submission has been received.' and provides a link 'Go back to the form'.


This page is displayed once you have submitted your form.

Step 3) Wait for 1-2 business days. Once your IP Address geo-location has been verified, you will receive an email from pulsedfrequency@pulsedfrequency.com notifying you that your login has been upgraded.

When you receive this email, login to your account and you will be able to download the professional version of the software.

Create an Account

If you do not have an account, select **I want to create an account**.

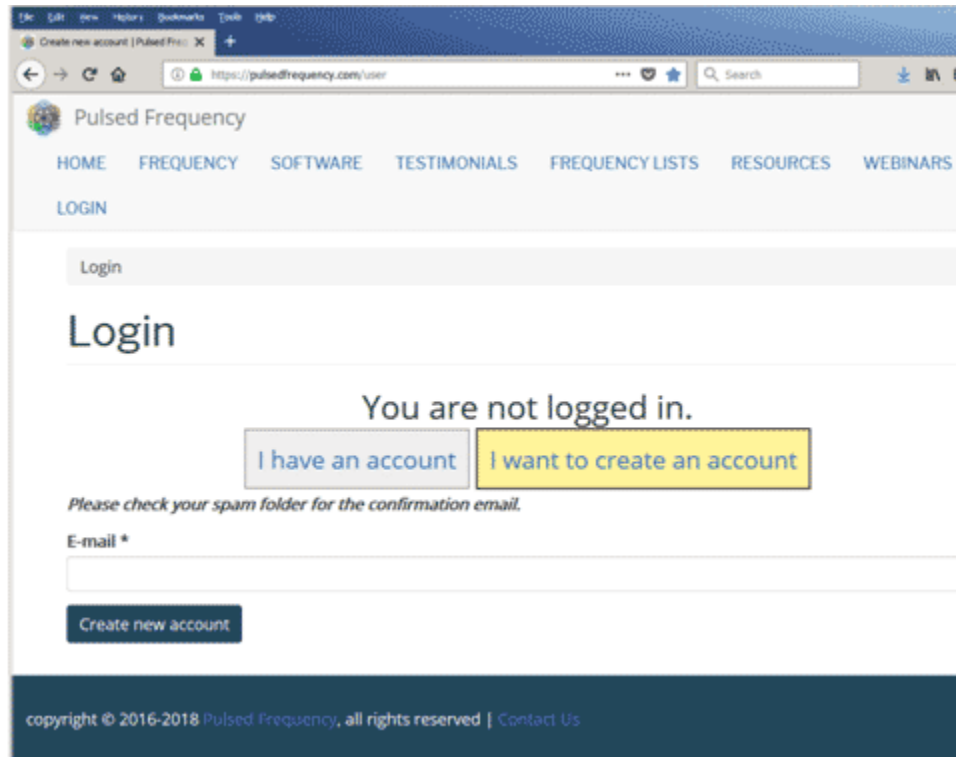

Enter your email address, then click **Create new account**. Further instructions will then be sent to your email address. The confirmation email will look something like this.

From: support@pulsedfrequency.com
To: rod@server.com
Cc:
Subject: Account details for rod_564 at Pulsed Frequency

Dear Registered User,

Thank you for registering at Pulsed Frequency. You may now log in by clicking this link or copying and pasting it to your browser:

<https://pulsedfrequency.com/user/reset/564/1534971011/JKZCwxsqdPQholdXsoli2wnP8Z5S4uiCxi-LJuTjH0>

This link can only be used once to log in and will lead you to a page where you can set your password.

After setting your password, you will be able to log in at <https://pulsedfrequency.com/user> in the future using:

username: rod@server.com
password: Your password

-- Pulsed Frequency team

Click on the link in the email and you will be taken back to the website to reset your password.

You have just used your one-time login link. It is no longer necessary to use this link to log in. Please change your password. ×

View

Edit

Orders

E-mail address *

rod@server.com

Password

Confirm password

Email updates

☒ Subscribe

Locale settings

Time zone

America/New York: Wednesday, August 22, 2018 - 5:06pm -0400

✓ Save

Enter a new password in both fields.

You have just used your one-time login link. It is no longer necessary to use this link to log in. Please change your password. ×

View

Edit

Orders

E-mail address *

rod@server.com

Password

•••••••• ✓

Confirm password

•••••••• ✓

Email updates

☒ Subscribe

Locale settings

Time zone

America/New York: Wednesday, August 22, 2018 - 5:06pm -0400


✓ Save

After you have changed your password, click the **Save** button. You will be told that the changes have been saved.


10

Download the Software

If you aren't already logged in, log into your account, then click the Software menu item.

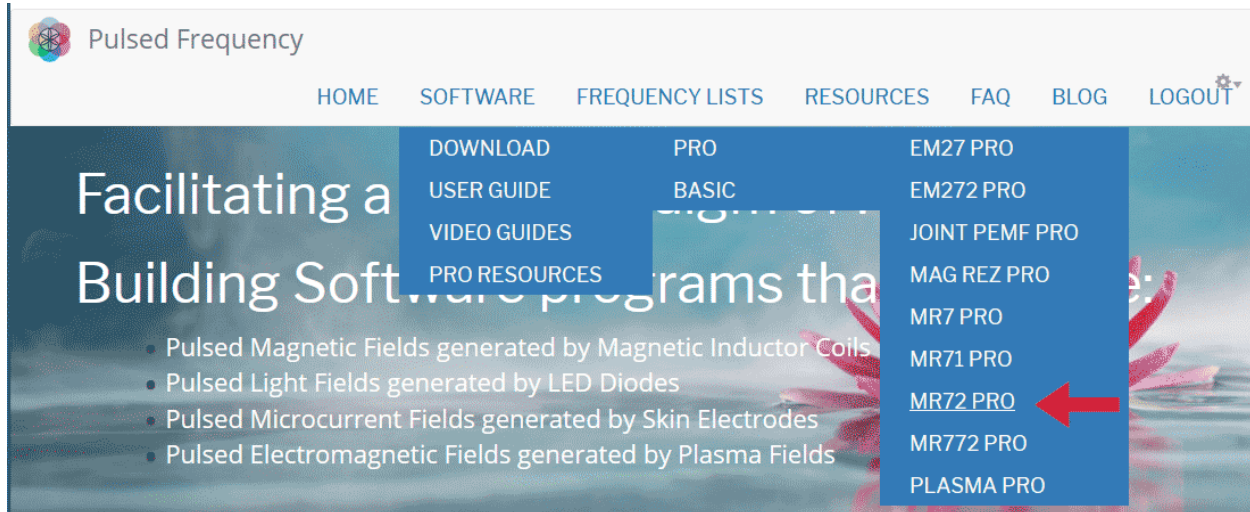


Next, point to **Download**, then click **MR72**. When you do this, you will be taken to the following page.

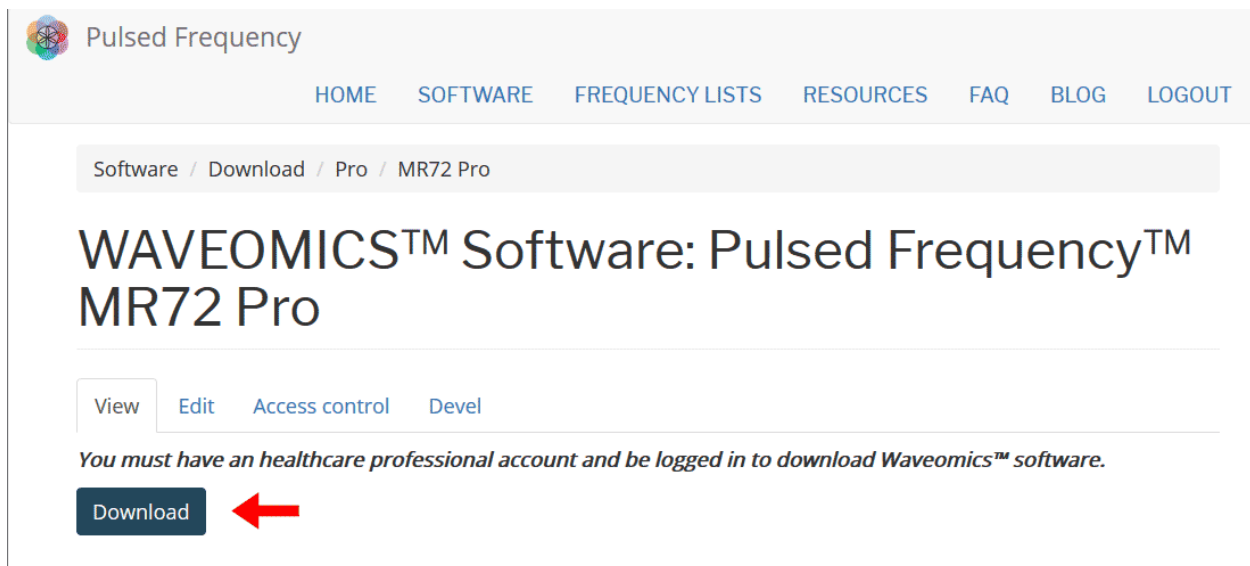


Click the **Download** button.

What happens next depends on the web browser you are using. Here are instructions specific to three different browsers being used today.

Chrome

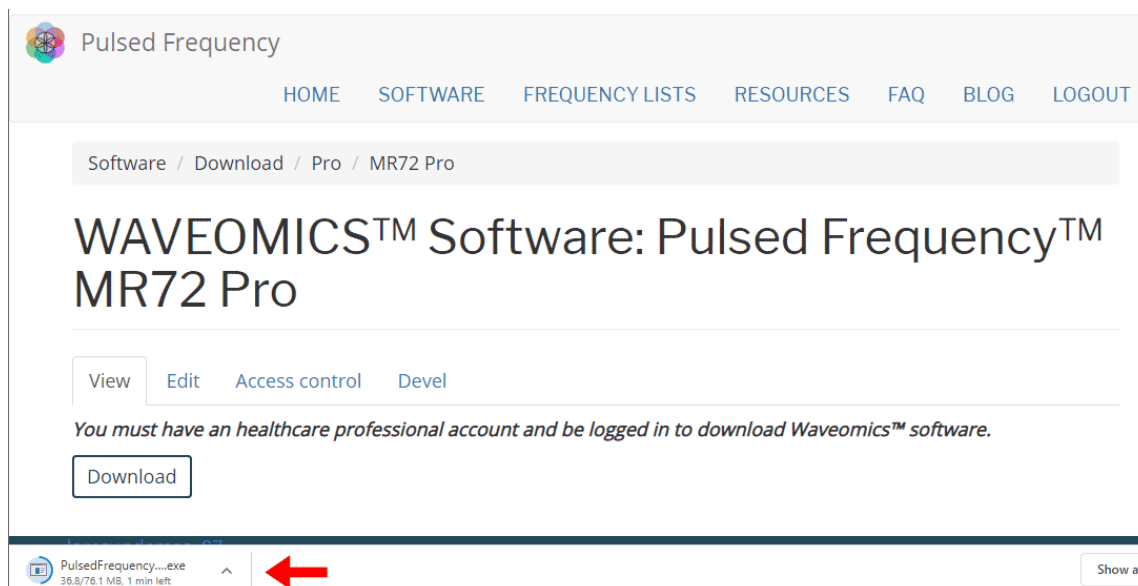


When you click the **Download** button, a notification displays in the lower left-hand corner of the browser that alerts you to the file being downloaded. You will see the number of bytes that have been downloaded and the total size of the file.

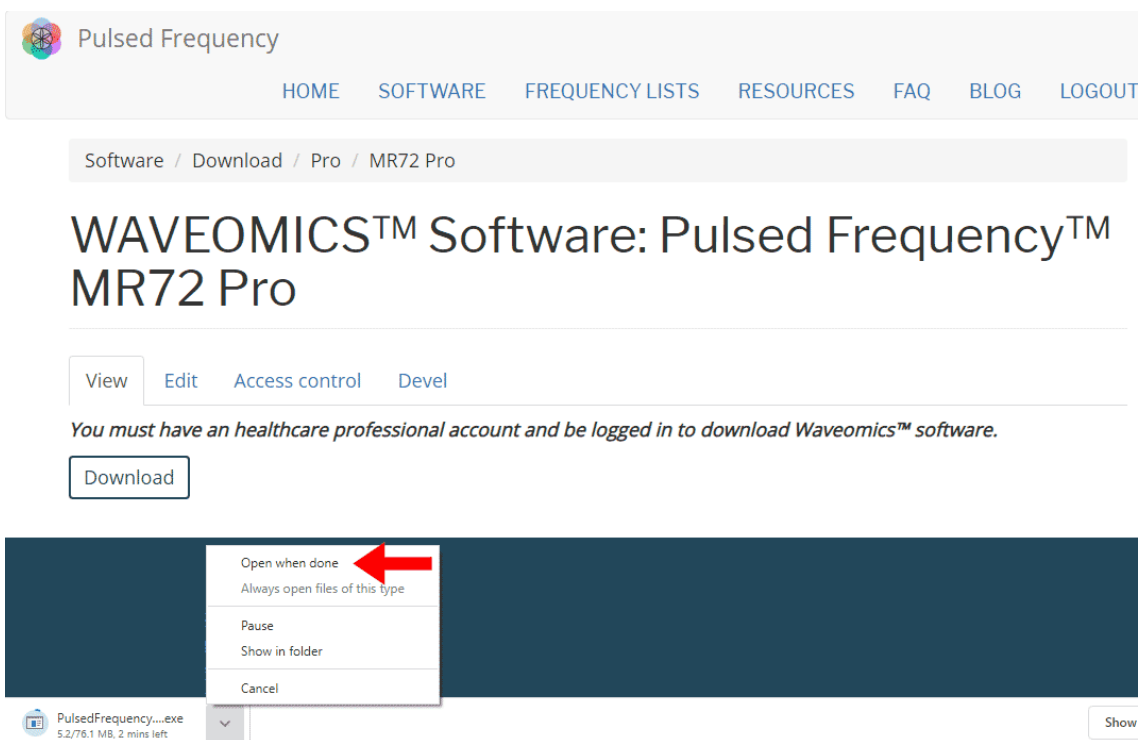


When the download has completed, click the down arrow and then click **Open when done**. This will run the installation program for the **MR72** software.


Firefox

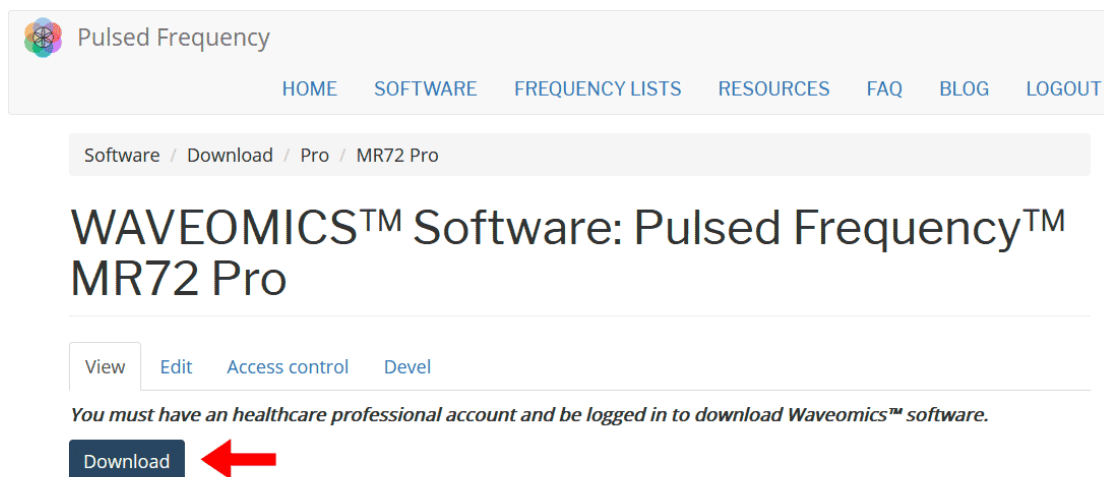


On this page, click the **Download** button and the following dialog box will pop up.

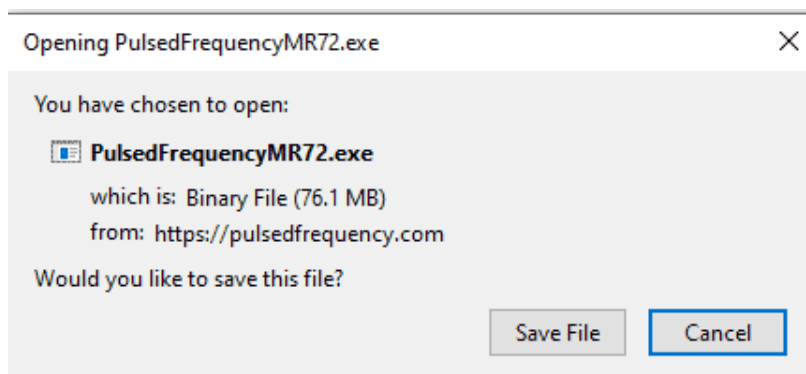


In this dialog box, click the **Save File** button.

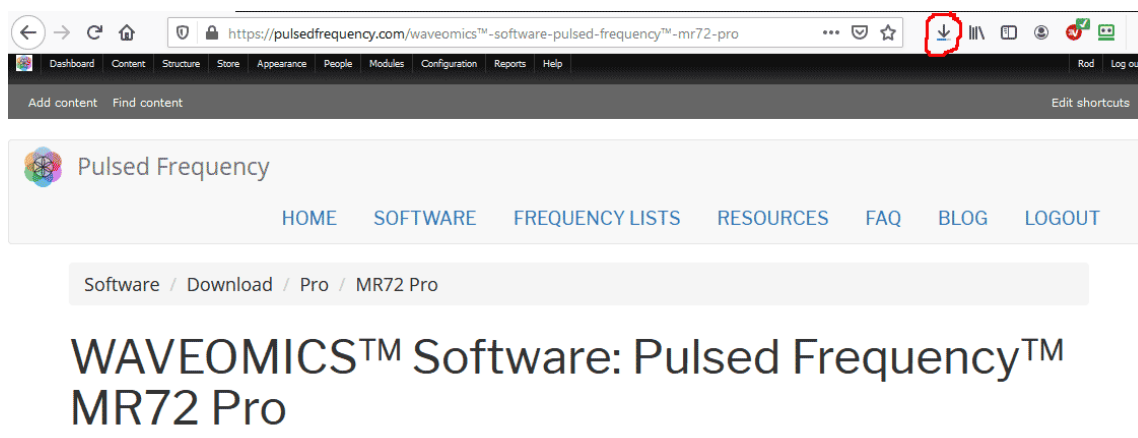

Next, go to the upper right-hand corner of the browser and click the **Down Arrow**.

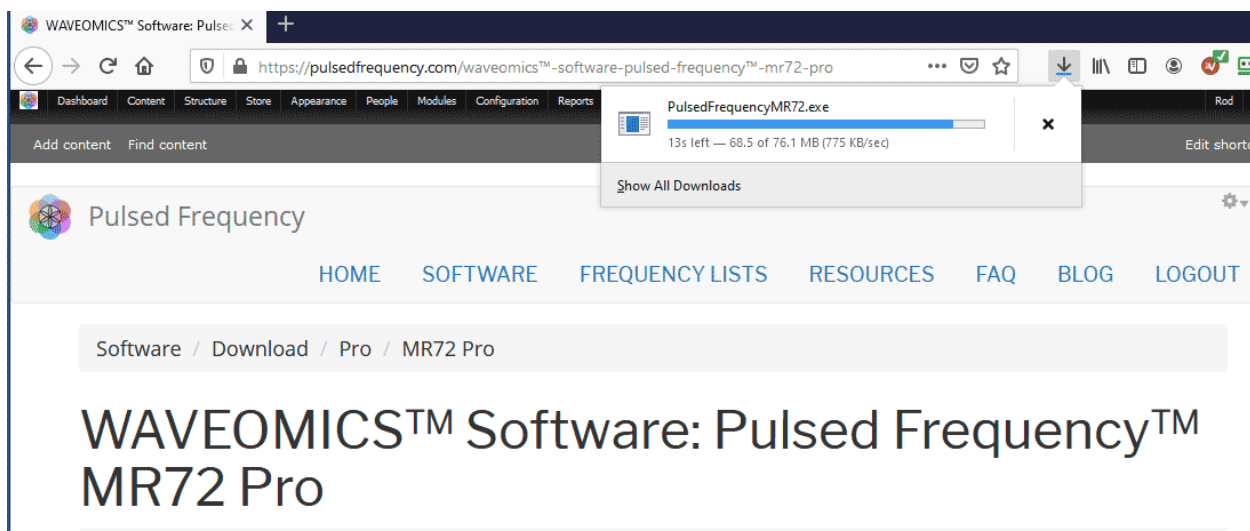


A small window will appear. Click the link in the lower left that says, **Show All Downloads**.

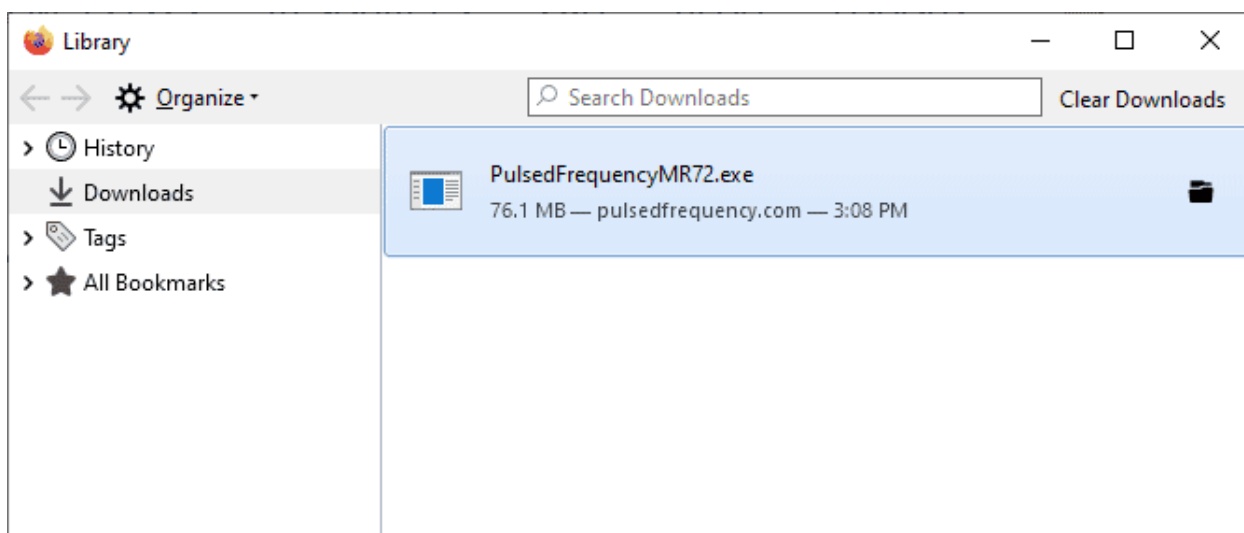


When the download has completed, the progress bar will disappear and you will see what is shown above. Double-click on the **PulsedFrequencyMR72.exe** file and the installation of the **MR72** software will begin.

Internet Explorer


When you click the **Download** button, a small rectangular window will display at the bottom of the screen.

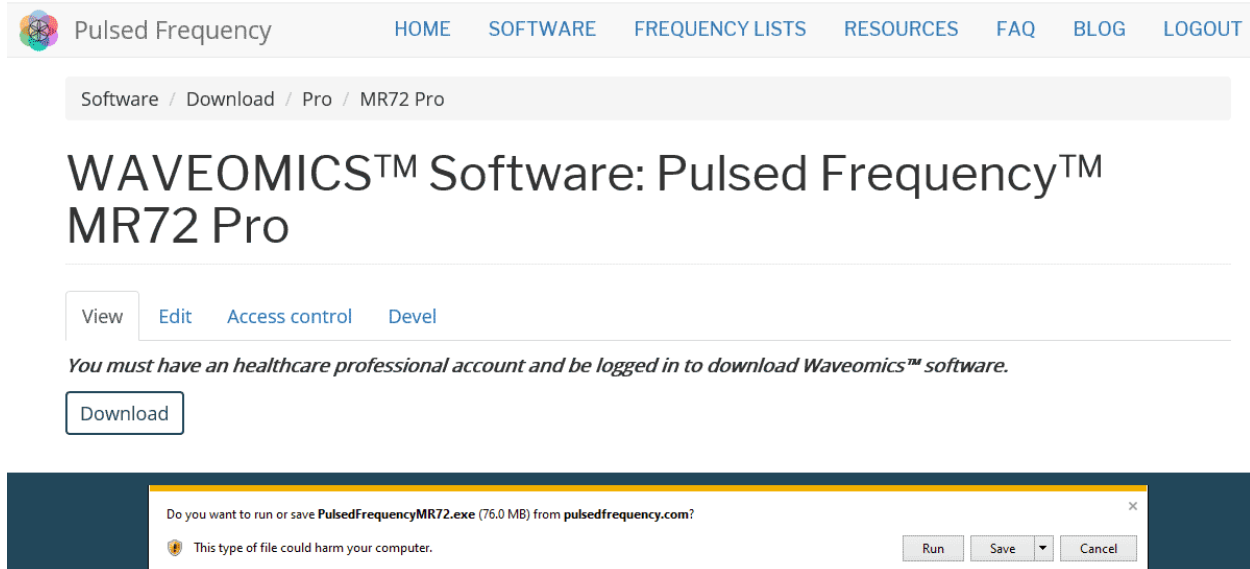

This window will show the progress of the file being downloaded.

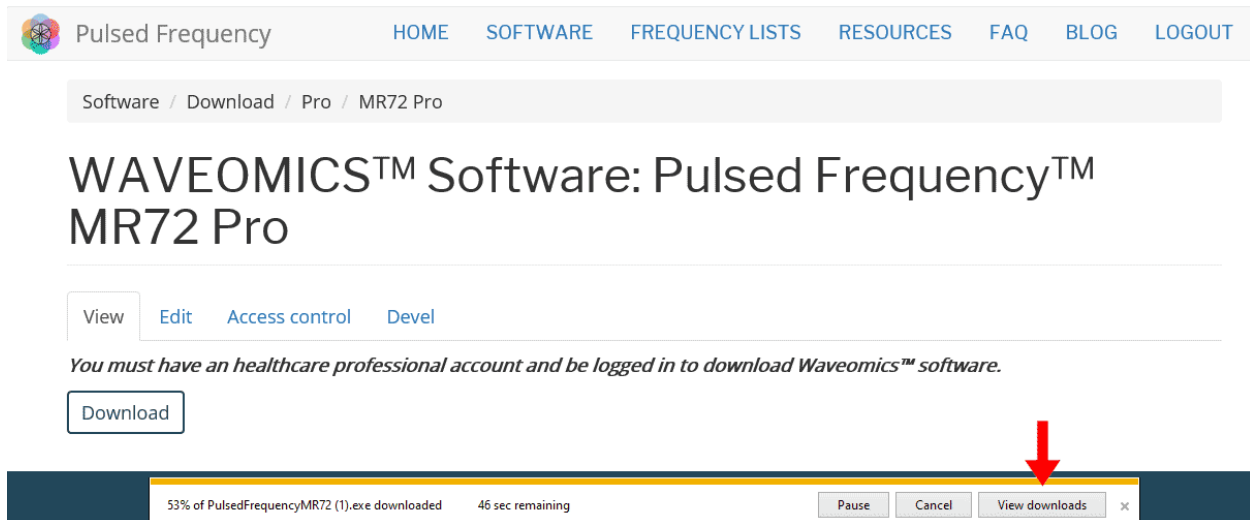


When file download has completed, click the **View Downloads** button.

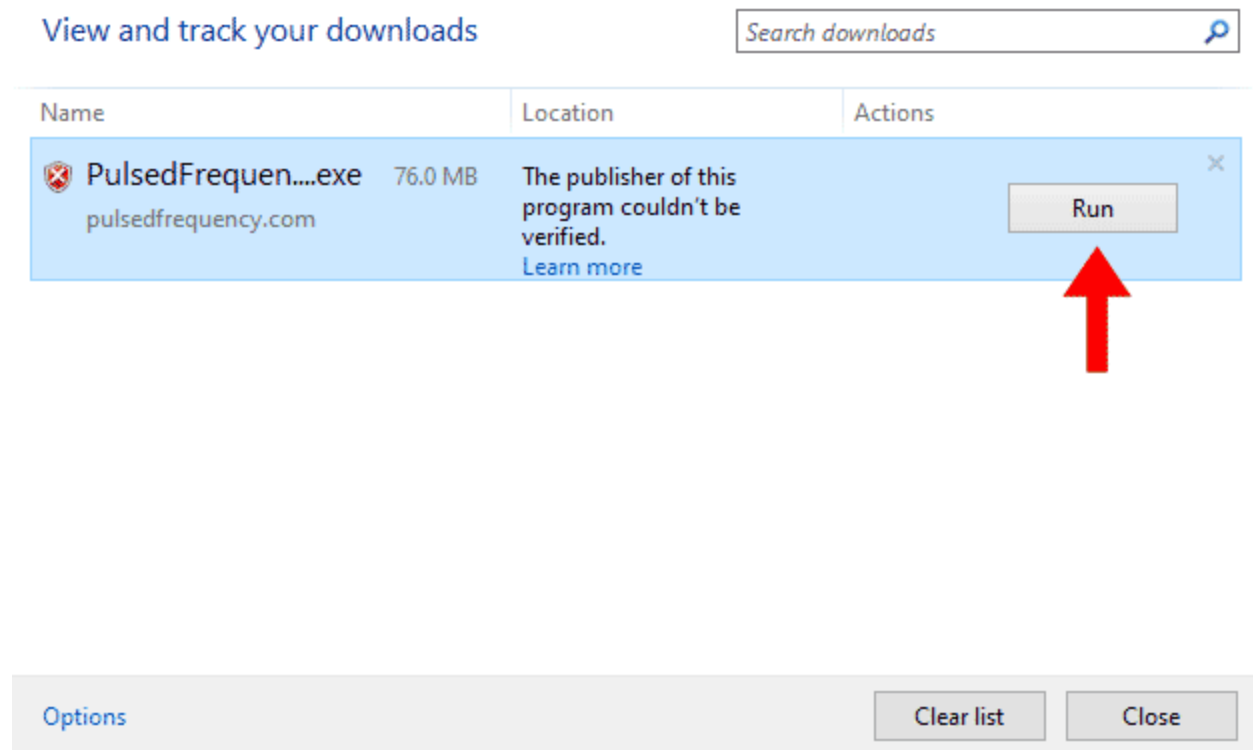


In this dialog box, click the Run button to run the **PulsedFrequencyMR72.exe** installation program.

Install the Software


To install the software, double-click on the downloaded file.

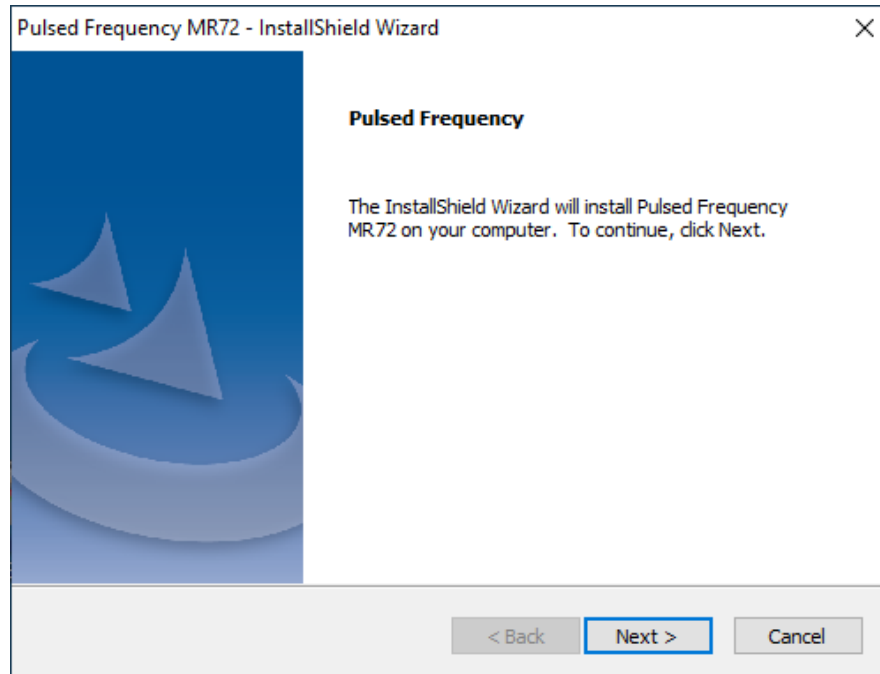


On this Welcome screen, click the **Next** button.

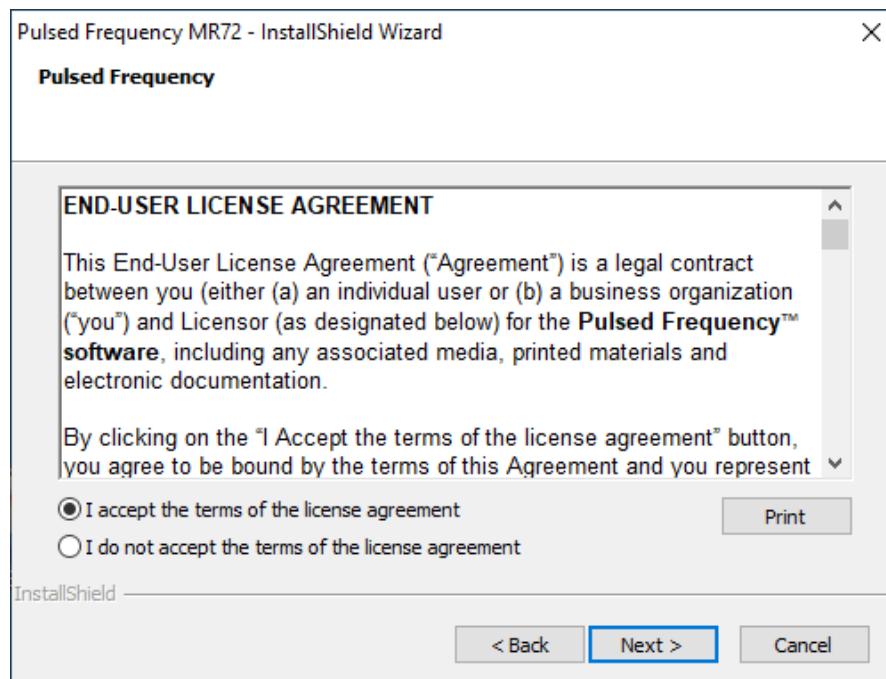


Click **I accept the terms of the license agreement**, then click the **Next** button.

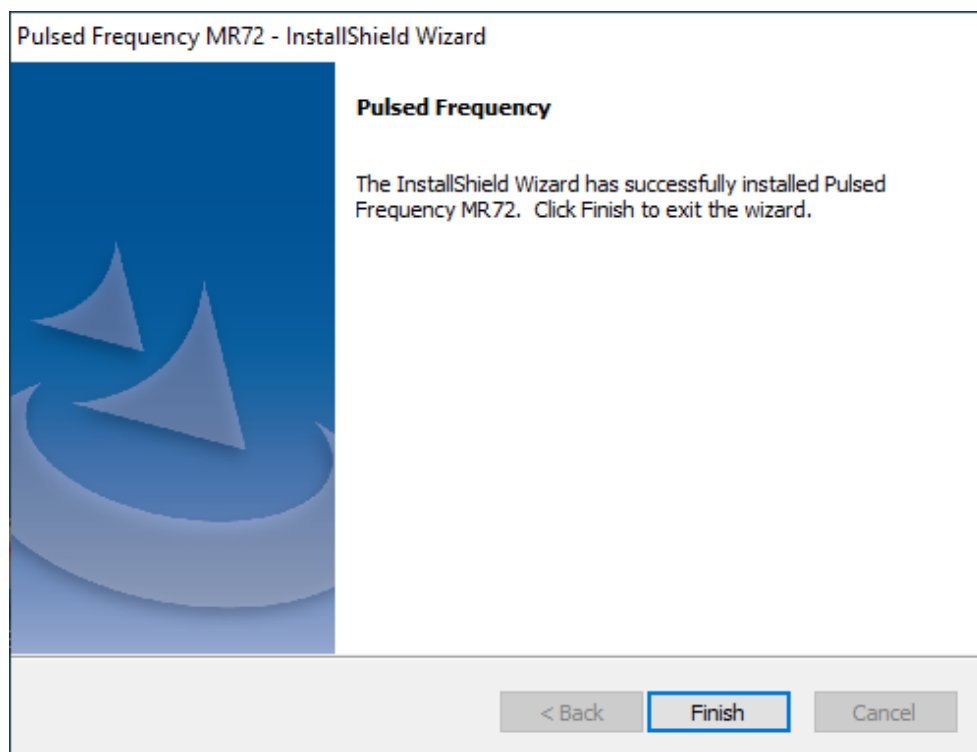


To begin the software installation, click the **Install** button.

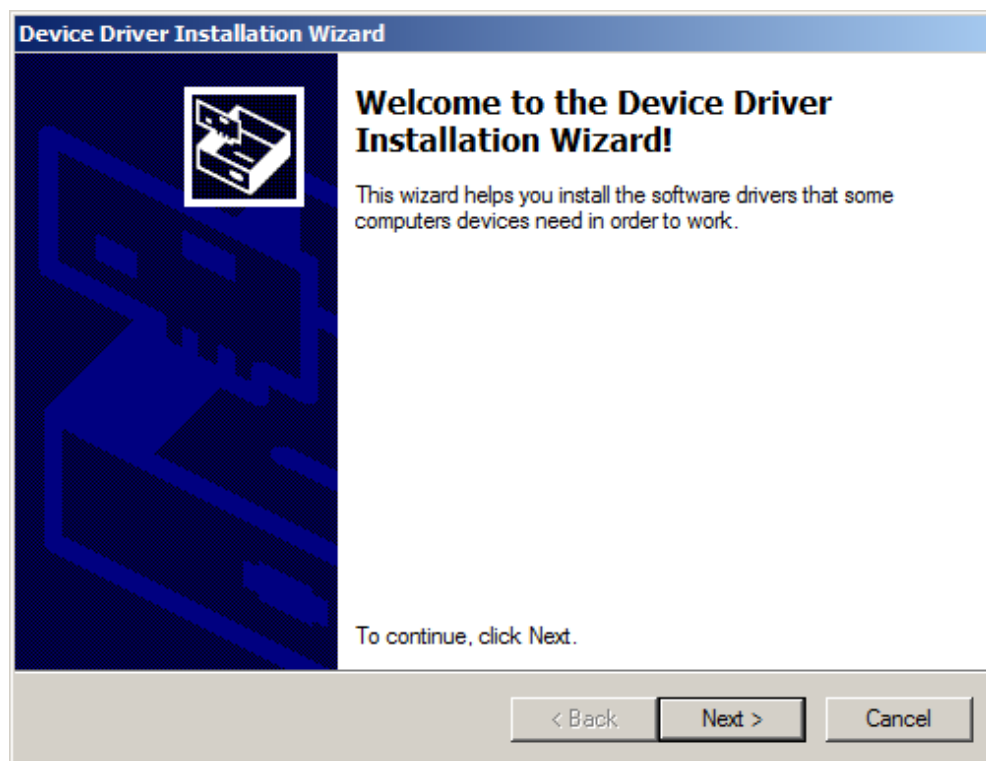


The drivers for your MR72 will be installed first. To proceed, click the **Next** button.

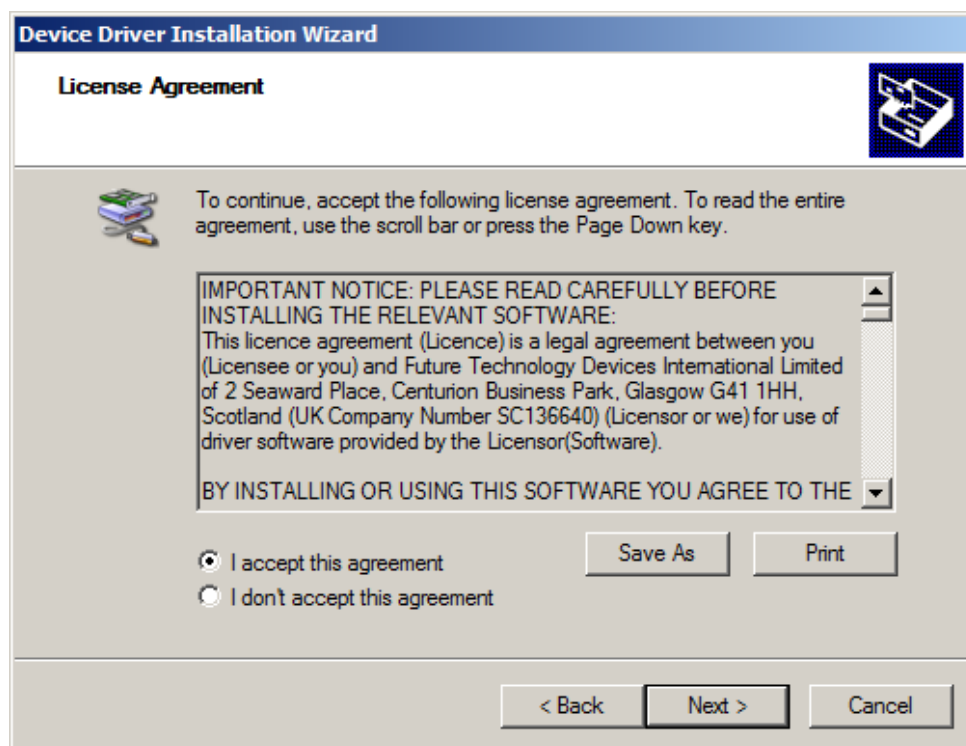


Accept the license agreement, then click the **Next** button.

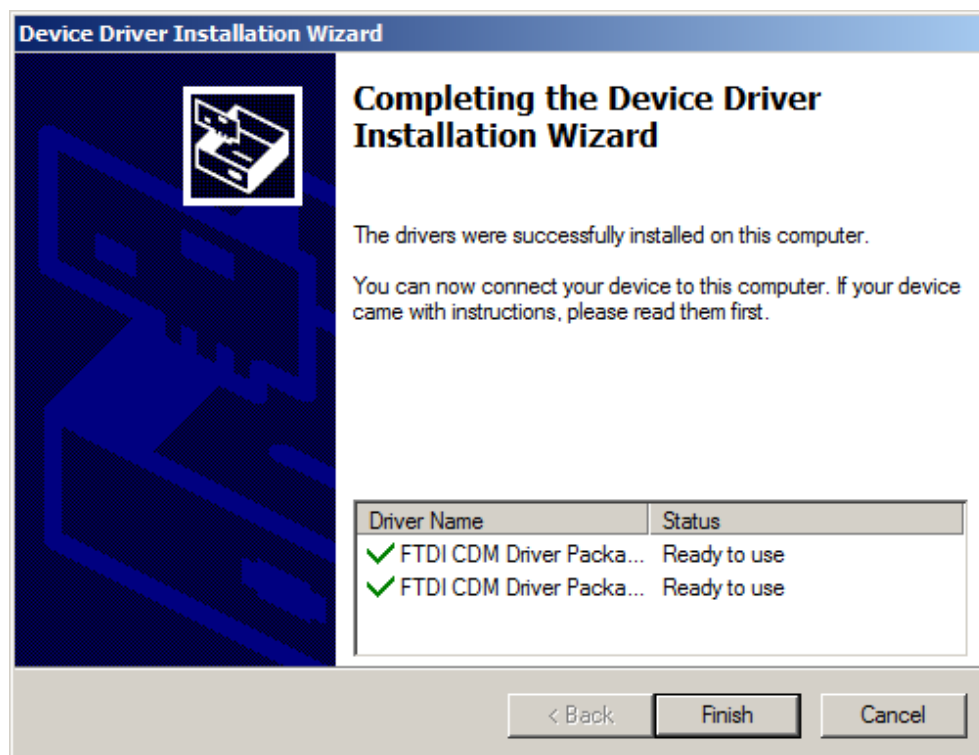


Click the **Finish** button to complete the driver installation.

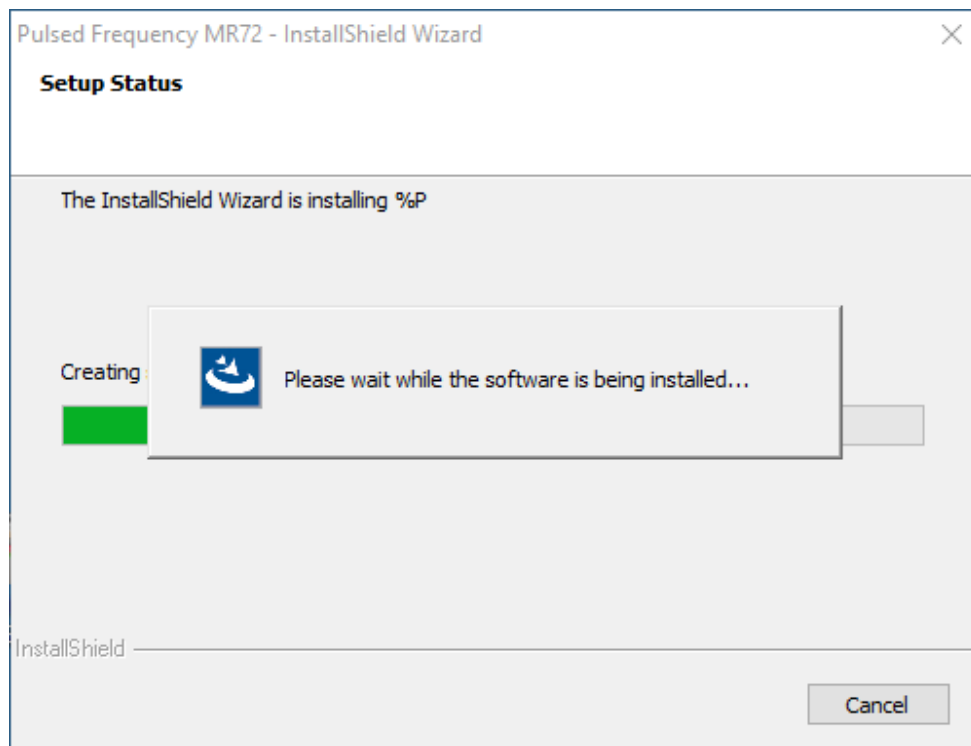

At this point, the Pulsed Frequency software will be installed. Just wait until it has completed.

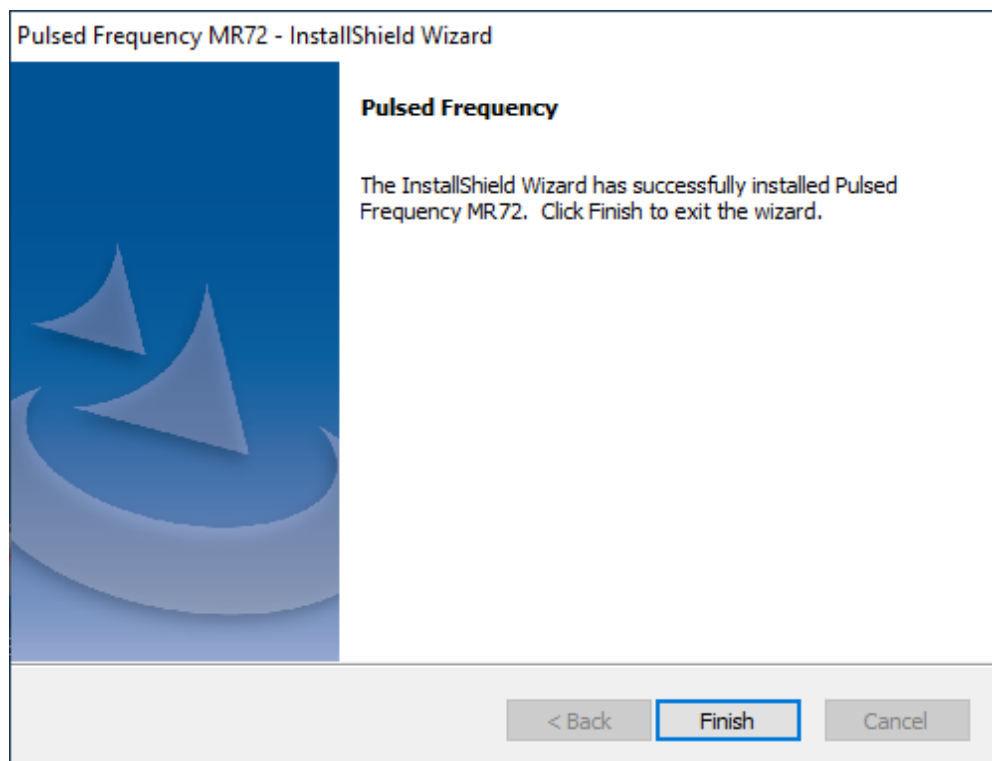

When you see this screen, the installation is complete. Click the **Finish** button.

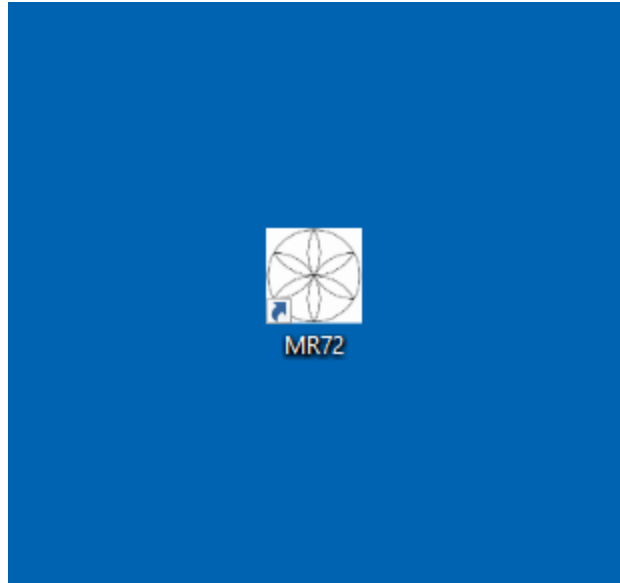

During installation, a shortcut to the MR72 software was placed on your desktop. You can double-click this shortcut to run the software.

Just Feel Better!

MR72 LED and Magnetic Pulsed Frequency Generator

The following steps are instructions for the MR72 Pulsed Frequency Generator. The device comes with a Frequency generator box, 2 LED pulsing light disks and/or 2 pulsing magnetic disks, and a 110 volt charger / power cord.

Setting up the MR72 Device

Insert the charger cable into the round port to the left of the On/Off button and the other end into a 110 volt electrical outlet. This will charge the device. A full charge will take approximately 4-8 hours. The light surrounding the On/Off button will flash Red/ Green when the charge is complete. The MR72 will run when the charger is connected or disconnected from the device. The MR72 device will run approximately 10 hours on battery power once charged.



To turn the MR72 device ON, Push the large On/Off button in the middle, until the lighted ring turns green. This ring will stay green while the programs are running. The Green On/Off light will turn Flashing Red when the device needs a charge. To turn the MR72 device OFF, press and hold the On/Off button for about two seconds. The device will beep and turn off. If running programs when the charger is plugged in, the green light will flash.



The MR72 offers the option of using Magnetic disks or LED light disks. If using the magnetic disks, it is suggested that you face the flower label side away from the body, so that you can see the flashing green lights on the flower. The magnetic pulses will go through clothing, so there is no need to have them against the skin. Unlike the LED lights.



The Magnetic disks or the LED disks plug into the RJ45 jacks on the back side of the MR72. Do not wrap the disc cables or Power cable around the MR72 device. Instead, unplug them and wrap each cable individually.

If using the two red LED light disks, plug them into the RJ45 plug jacks on the bottom of the MR72. When using the LED lights, the lights MUST face the skin. The lights will not penetrate through cloth. The LED lights will feel warm. The lights need to breathe. Do not sandwich them between you and furniture. If the LED lights get too warm for your skin, move to another position. LEDs can be held against the skin with a brace, sock or ace bandage.



The MR72 device has the ability to be reprogrammed. To the right of the On/Off switch, there is a mini USB port. You will need to use a USB/ Mini USB cable to connect the unit to your computer if you want to transfer programs. Programs and the appropriate software can be obtained from www.Pulsedfrequency.com.



You may find it convenient to use the LEDs against your body during the day, then use the Magnetic disk under your fitted sheet at night, so that you can sleep on top of them. This regimen will maximize the treatment effect. You may also tuck the MR72 device and the two magnetic disks into a brace around a knee or other joint.

MR72:Useful Tips

It's very important to drink a minimum of 32 ounces of purified water before a treatment, and another 32 ounces of purified water after the treatment. The water helps the frequencies flow through the body and cleans out the debris that the cells are casting off.




You may experience a slight dizziness or detoxing flu-like effects from this treatment. If this happens, reduce the treatment time. Slowly increase daily treatment time until all programs are run and the unit shuts off. Also increase your water intake until symptoms subside.

It is suggested not to use electronic devices while being treated, such as computers, cell phones, I-pads and Kindles. Electronic devices may not work within the electro-magnetic field. This caveat does not apply to LED Lights.

Disclaimer: The MR72 device does not claim to treat or correct any medical diseases, injuries or symptoms. The MR72 device is considered to be Wellness device.

Connect MR72 to Your Computer

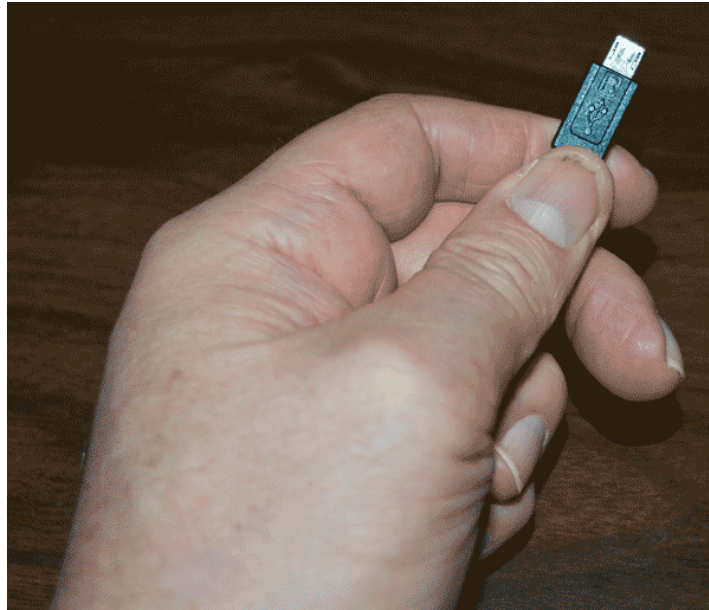


To connect the MR72 to the computer, take the supplied Mini-USB cable and orient the smaller end so that it can be plugged into the device.



Make sure the MR72 is OFF and plug the Mini-USB cable into the mini-USB jack in the unit. The MR72 is OFF if the green LED ring light is not lit.




Plug the larger end of the USB cable into your computer.

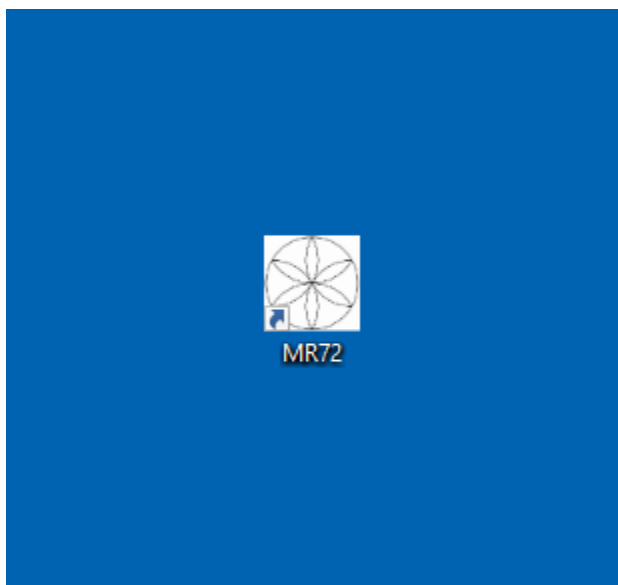


To run the MR72 software, double-click the **MR72** shortcut on the desktop.

Run the Software for the First Time


When you first run the software, it will check to see if file bank and software updates are available. This will also happen any other time you run the software.

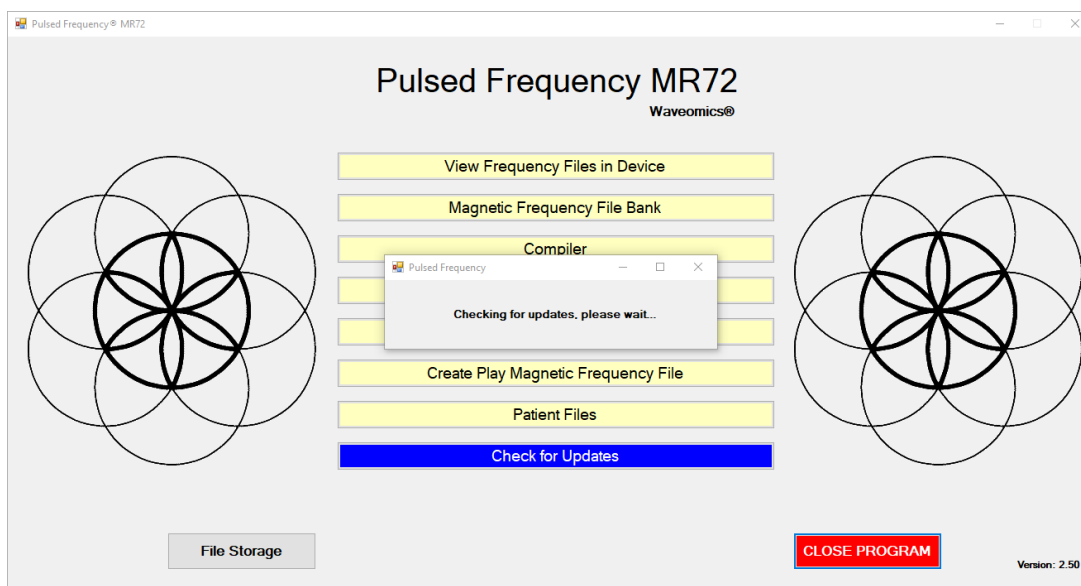


During this process, a small dialog box will display. If no updates are available, the dialog will just go away.

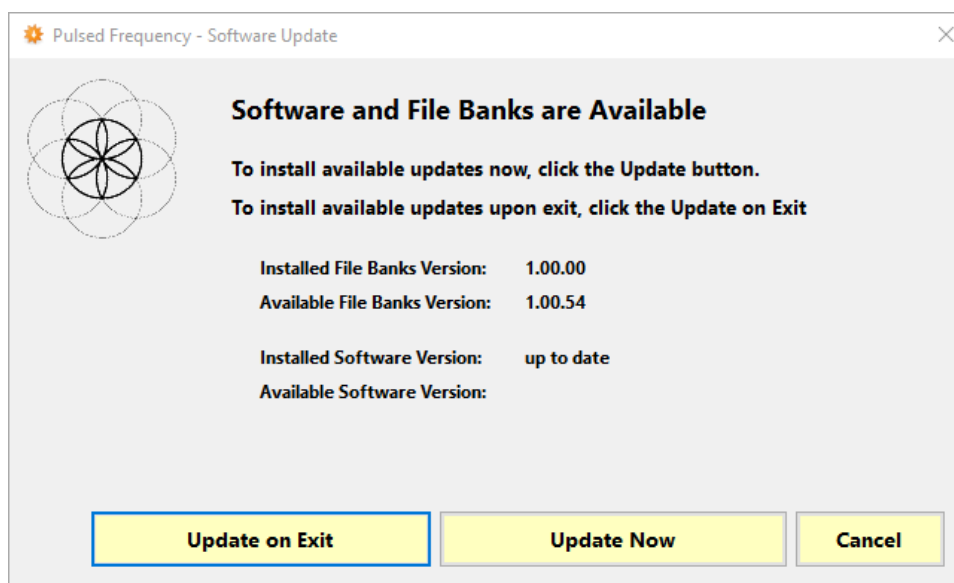

If updates are available, the above dialog box will appear. If you click **Update on Exit**, this box will disappear and you will be back at the main menu page. The software will then be updated when you click the **Close Program** button. If you click **Update Now**, the software will be updated immediately. If you click **Cancel**, no update will be performed.

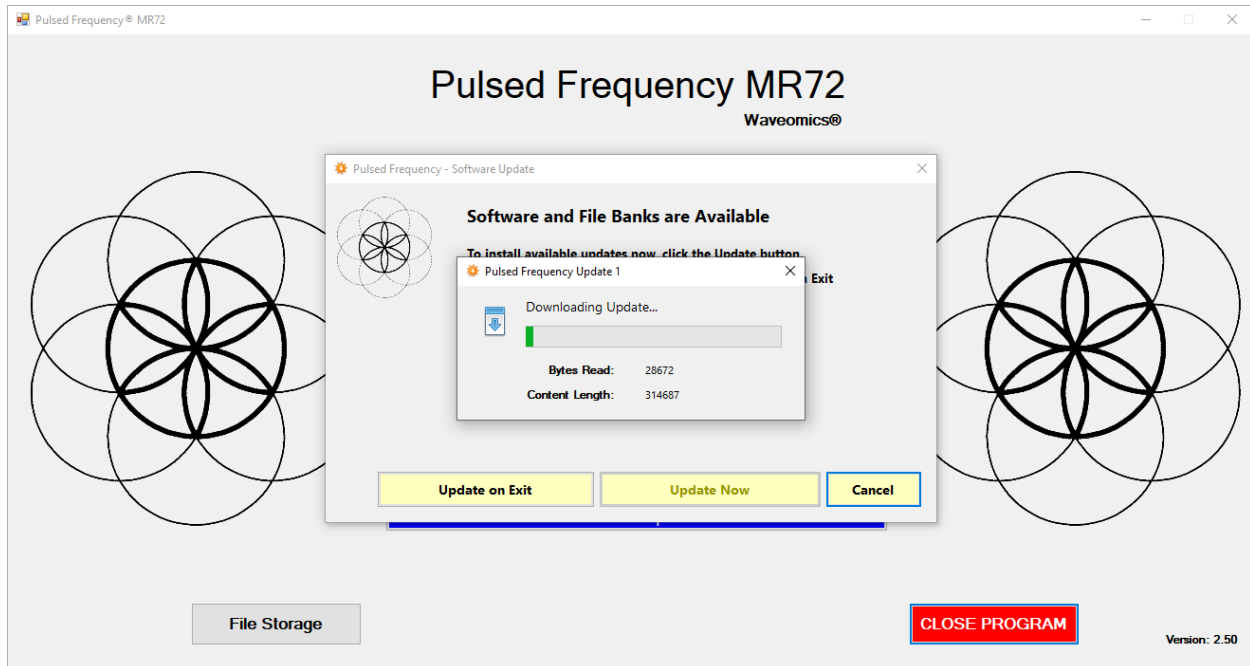


If you clicked **Update Now**, a progress bar will be displayed as the software and file banks are being downloaded.

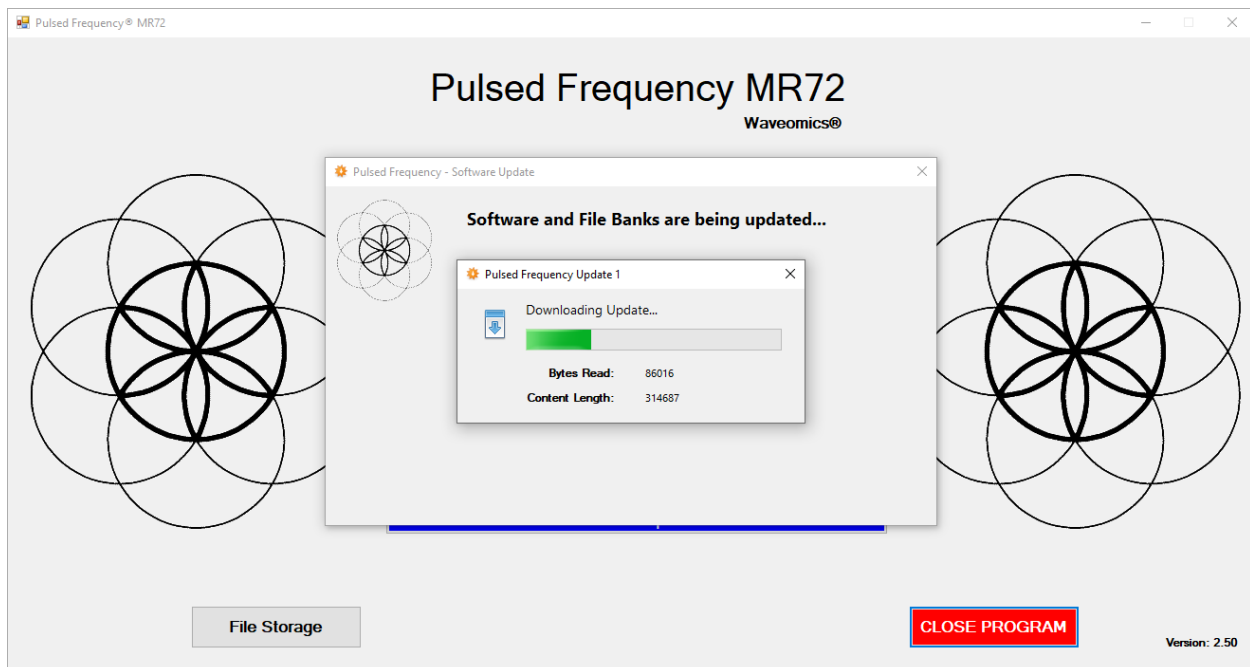

If you clicked **Update on Exit**, the above dialog box will be displayed when you click the **Close Program** button.

After the software has been updated, you can use any of the functions on the main menu page. However, if this is your first time using the software, click the Compiler button.

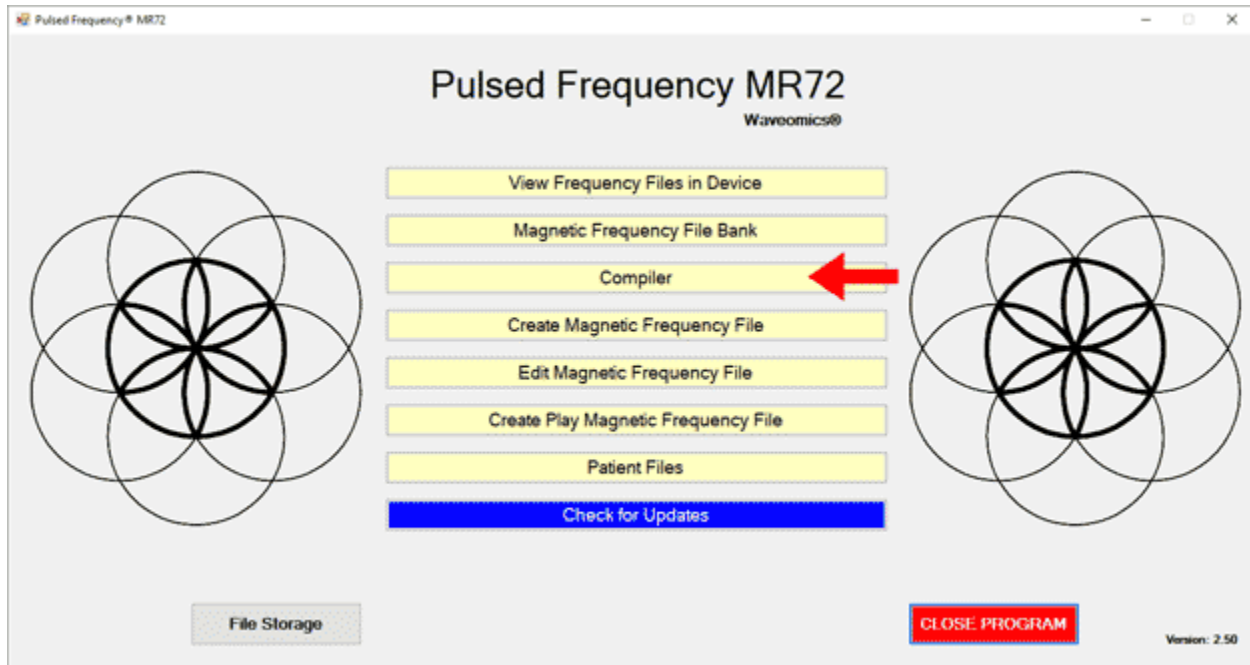

Compiler

The Compiler allows you to load treatment programs into the MR72.

Pulsed Frequency® MR72

Compiler

Waveomics®

Categories

- ☒ A-Z All Files
- ☐ A-Z Combined
- ☐ Compiled Files
- ☐ Wellness
- ☐ Allergy
- ☐ A-Z New Files
- ☐ Blood
- ☐ Breast
- ☐ Cardiovascular Lymph
- ☐ CNS Balance
- ☐ CNS Behavior
- ☐ CNS Brain
- ☐ CNS Concussion
- ☐ CNS Cord
- ☐ CNS Degen Path
- ☐ CNS Headache
- ☐ CNS Movement
- ☐ CNS Pain
- ☐ CNS Stroke
- ☐ Cysts Ganglion
- ☐ Dental
- ☐ Ear

Frequency Files (# of freq rows)

- ☐ Abdominal Adhesions Est 58 (9)
- ☐ Abdominal Hernia Est 58 (7)
- ☐ Abdominal Hernia Test VG Est 1 (1)
- ☐ Abdominal Hernia VG Est 190 (7)
- ☐ Acetylchol Tx Est 60 (14)
- ☐ Acne Est 30 (6)
- ☐ Acute Injury Est 452 (117)
- ☐ ADD ADHD Est 132 (30)
- ☐ ADD ADHD Est 60 (13)
- ☐ Adipose Lipoma Est 60 (9)
- ☐ Adrenal Cortex Quiet Est 40 (7)
- ☐ Adrenal Cortex Support Est 35 (5)
- ☐ Adrenal Medulla Quiet Est 40 (7)
- ☐ Adrenal Medulla Support Est 54 (11)
- ☐ Adrenal Support VG Est 22 (18)
- ☐ Allergy Est 40 (7)
- ☐ Allergy General Inflammation Est 32 (9)
- ☐ Amp Hand Post Op Est 60 (20)
- ☐ Anal Scarring Est 60 (11)
- ☐ Anal Scarring VG Est 47 (28)
- ☐ Anesthesia Removal Est 33 (4)
- ☐ Ankylosing Spondylitis Est 50 (11)

Compiled Frequency File Name

Number of Repeats (Max 255)

Play Order	Frequency File	Time	Delete

Total Number of Minutes (Max 999)

Total Number of Rows (Max 500)

Add →
Delete Frequency File

Save Compilation
without Transferring

Transfer Treatment to Device

[Return to Home Page](#)

There are several categories of treatment programs available in the Compiler. Here are the major categories that always appear at the top of the **Categories** list.

- ☐ **A-Z All Files** - an alphabetical listing of all treatment files in all categories.
- ☐ **A-Z Combined** - a list of compiled treatment programs that you have created.
- ☐ **Commonly Used Compiled Files** - a list of predefined treatment programs supplied with the software that are for specific purposes.

Treatment programs can be created in two ways. You can create your own treatment program or select a predefined program.

To select a predefined program, under **Categories**, click the **Commonly Used Compiled Files** category. Next, under **Frequency Files**, click one of the predefined programs, then click the **Add** button. When you do this, the files in that treatment program will be loaded into the spreadsheet on the right.

To create your own treatment program, just select a treatment file from one of the categories and click **Add**. Repeat this process until you are finished. The software will allow up to 999 minutes of total programming.

Compiler Waveomics®

Compiled Frequency File Name: Concussion Est

Number of Repeats (Max 255): 0

Play Order	Frequency File	Time	Delete
1	Concussion Brief Est 10	10	X
2	CNS Forebrain Acute Est 30	30	X
3	Reset CNS Est 50	50	X
4	CNS Medulla Acute Est 30	30	X
5	Brain Fog Est 30	30	X
6	PTSD Stress Est 60	60	X

Total Number of Minutes (Max 999): 210

Total Number of Rows (Max 500): 55

Save Compilation without Transferring

Transfer Treatment to Device


Return to Home Page

In the example above, we selected Concussion Est 210, then clicked Add.


After you have selected the treatment programs, you must enter the Number of Repeats. If you want the set of programs to run one time only, enter a 0 for the Number of Repeats. If you enter 2 for the repeats, the set of programs will run once, then repeat two more times, for a total of 3 times. You may enter a number of repeats from 0 to 255.

When you are ready, click the **Transfer Treatment to Device** button and the Name Bank list will be displayed. Every time a treatment is transferred to the EM272, you will need to select a person's name under which to file it. The treatment will then be saved to that person's treatment file history in the Treatment Files function that is accessed from the main menu page.

If you do not see the Name Bank list, the following message will probably be displayed. This means you have a connection problem.

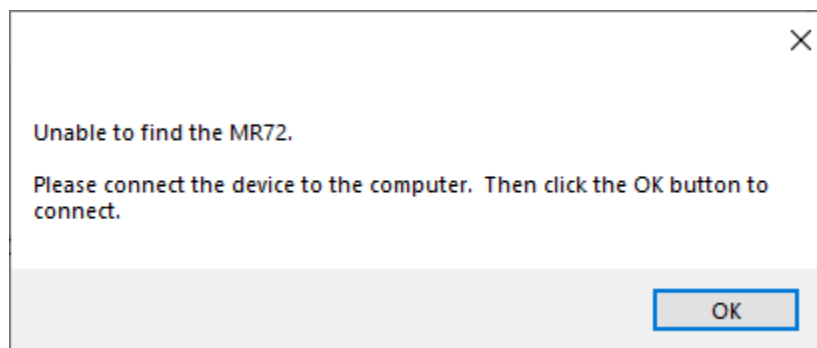


When this happens, go to the **Troubleshooting** section of the manual.

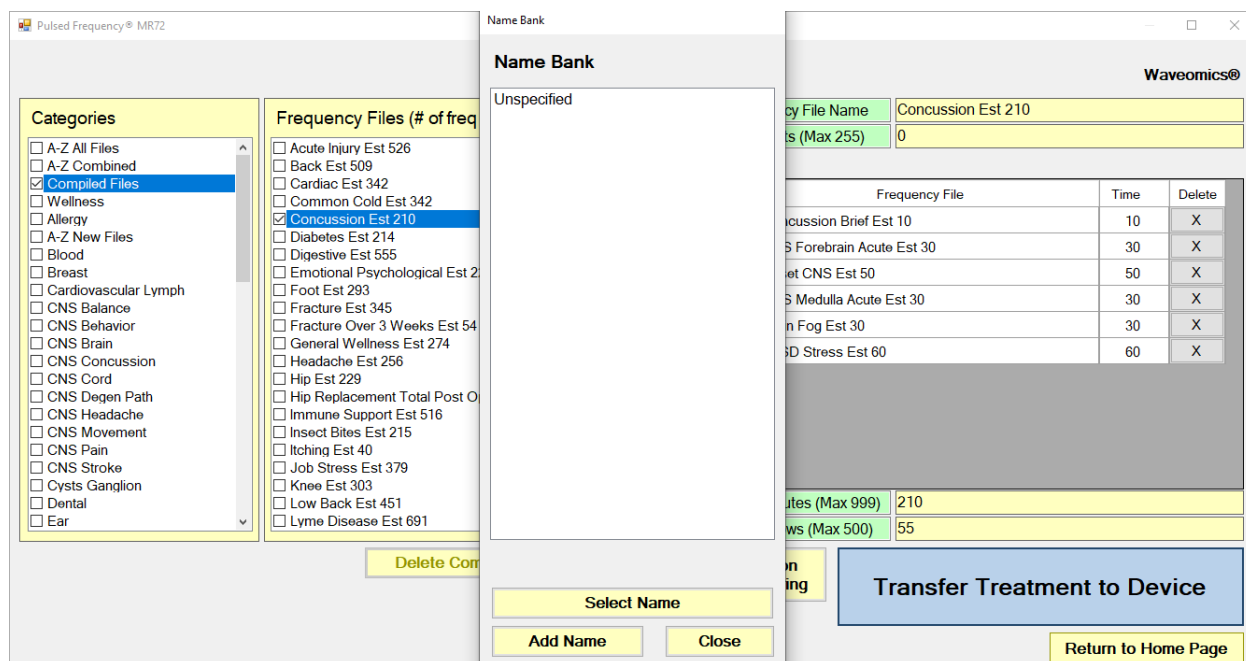


If you have no connection problems, the Name Bank list will be displayed. Just select any name from the list. You can also create a new name to associate with the treatment.


To create a new name, click the **Add Name** button.

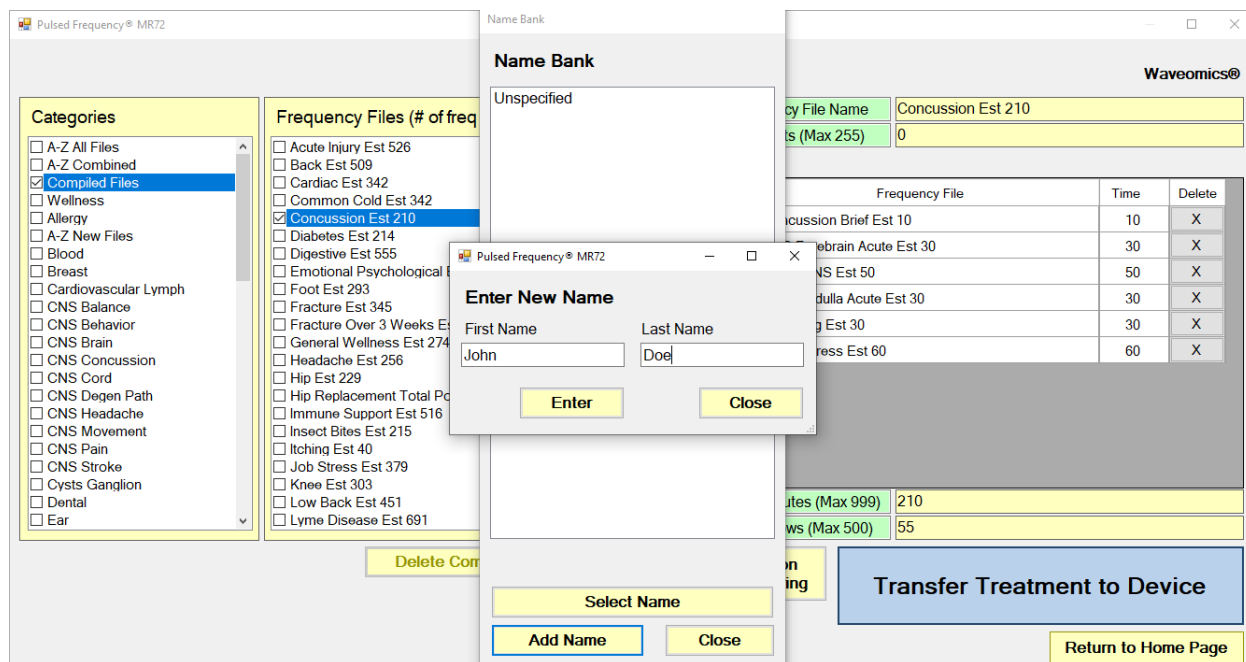

Enter a First Name and Last Name, then click the **Enter** button.

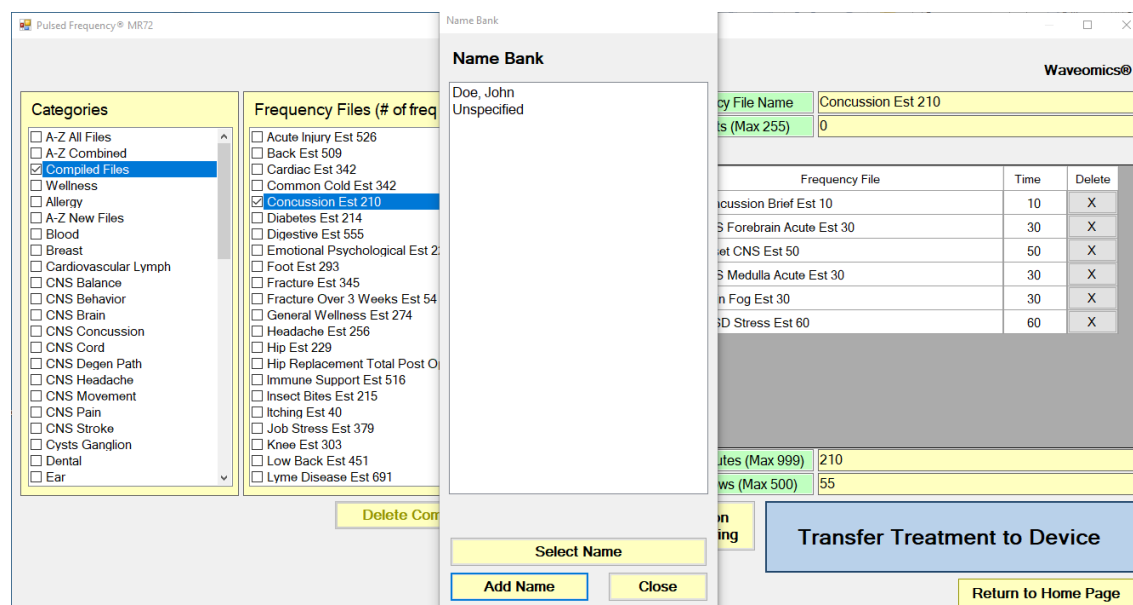

The new name will appear in the list. Select that name and the treatment files will then be transferred to the MR72 device. As this is taking place, the software will switch to a different screen.

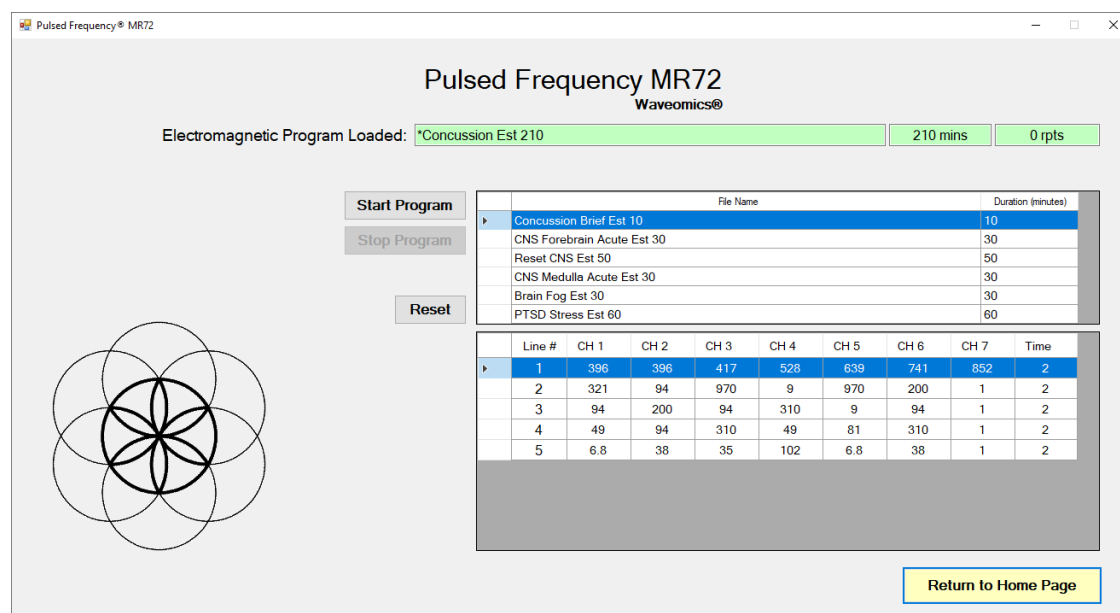


This screen is the same one as is displayed when you click the **View Frequency Files in Device** button on the main menu page.

At this point, the MR72 device has been loaded and is ready to use. For most people, you will use the device in standalone mode by exiting from the software, disconnecting the USB cable from the device and turning the unit ON. However, if you are a practitioner, you will generally Start and Stop the play of the device from the above screen. This is explained in the section of the manual entitled, **View Frequency Files in Device**.

Main Menu

When you run the software, the main menu page appears.

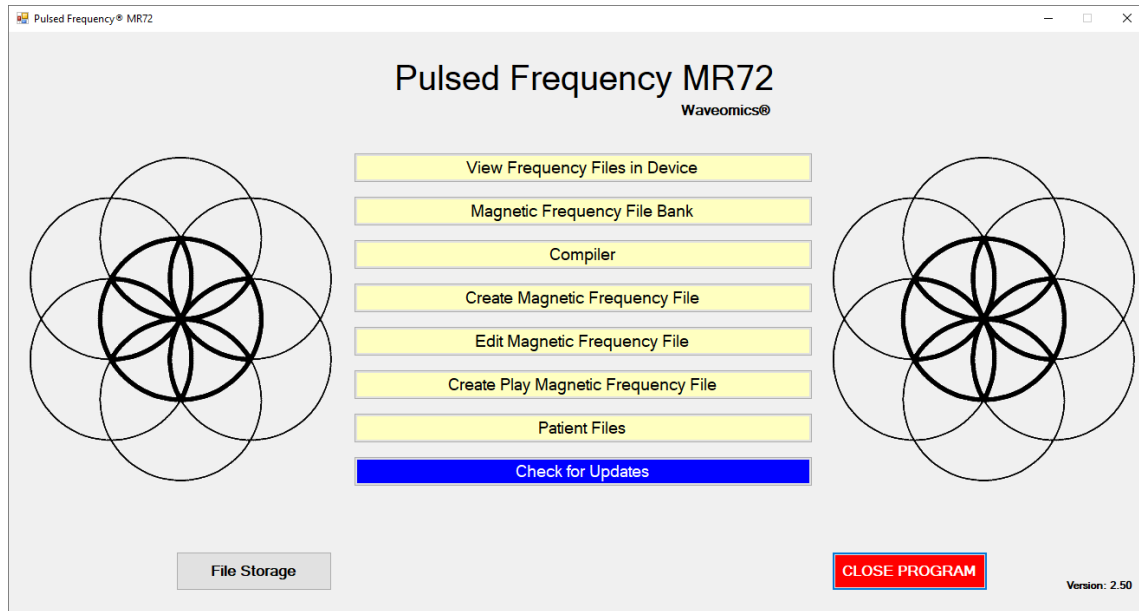


Here are all the functions available from the main menu page.

- ☐ **View Frequency Files in Device** - This allows you to view the frequency files currently loaded into the MR72.
- ☐ **Magnetic Frequency File Bank** - This allows you to view the frequencies in any frequency file in the frequency file bank.
- ☐ **Compiler** - This allows you to build treatment programs and transfer them into the MR72.
- ☐ **Create Magnetic Frequency File** - This allows you to create a frequency file from scratch and save it.
- ☐ **Edit Magnetic Frequency File** - This allows you to edit an existing frequency file and save it.
- ☐ **Create Play Magnetic Frequency File** - This allows you to test frequencies one row at a time.
- ☐ **Treatment Files** - This allows you to view a history of treatments that have been loaded onto the MR72 in the past. You can select any one of them and load it again into your device. You can also print any part of the treatment history you wish or save it to a text file.

- **Check for Updates** – This checks to see if software and file bank updates are available.
- **File Storage** - This allows you to indicate where to save your treatment files. It can also show you the serial number of your MR72 device, and allow you to choose what type of device detection method to use.


View Frequency Files in Device

When you select this function, you can view the frequency files loaded into the MR72.

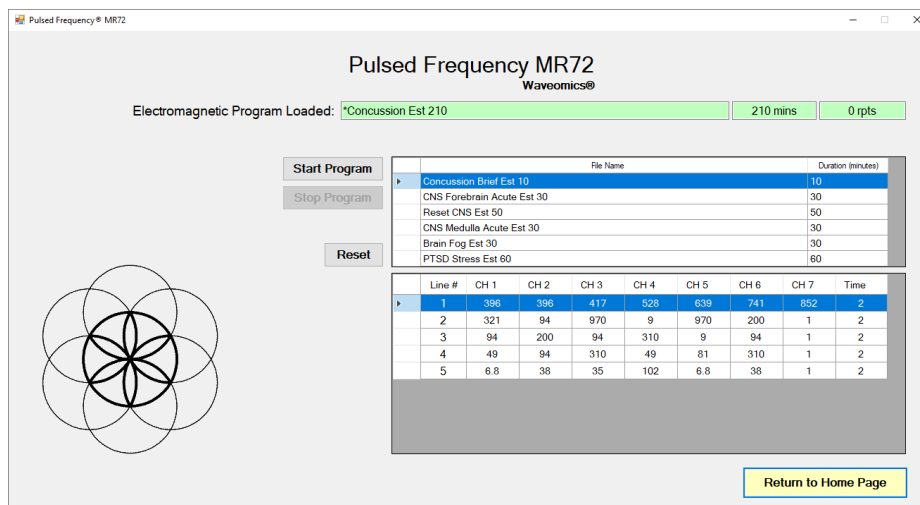

This screen shows the name of the treatment program that is loaded, the total running time of the treatment and the number of repeats.

If you do not see any treatment files, but rather see the words, "MR72 is not connected", then you have a connection problem and need to diagnose it by going back to the **Connect MR72 to Your Computer** section and follow the instructions.

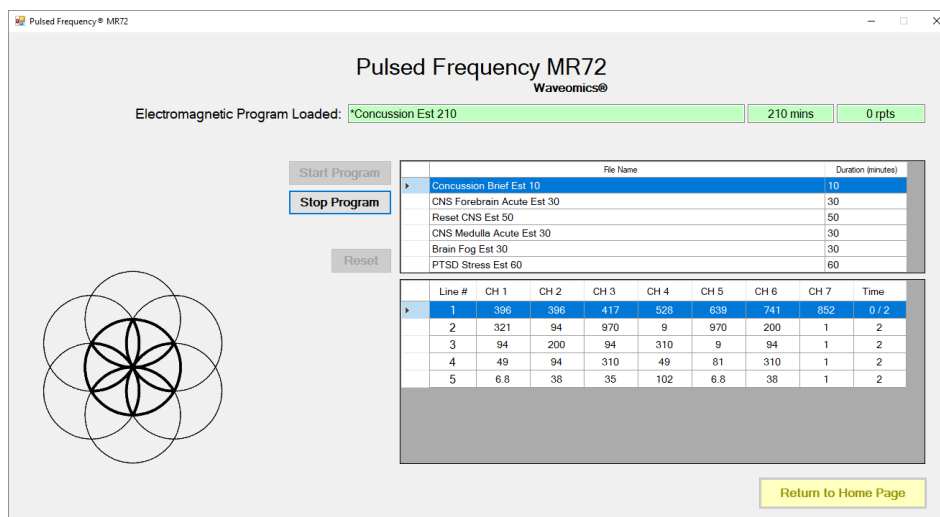

This screen also allows you to start and stop the play of frequency files that are loaded onto the device. With the MR72 connected to your computer, click the **Start Program** button. The MR72 will turn ON and play frequencies starting with the first row of the first file. This will continue to take place until all files have been played. When you loaded the files onto the device, if you entered a number of Repeats greater than 0, then the entire sequence of files will

start to play again, all the way through, for the specified number of repeats. After this process has finished, the MR72 will stop playing.

You can stop the play of frequency files at any time by clicking the **Stop Program** button.

The **Reset** button allows you to set the current file and current row back to the beginning of the sequence of files (first row of the first file).

Pulsed Frequency MR72
Waveomics®

Electromagnetic Program Loaded: *Concussion Est 210 210 mins 0 rpts

Start Program
Stop Program
Reset

Line # CH 1 CH 2 CH 3 CH 4 CH 5 CH 6 CH 7 Time


1	200	94	970	124	321	9	49	4
2	7.8	396	417	528	639	741	852	4
3	40	89	90	94	84	10	709	6
4	40	562	102	310	71	33	288	6
5	284	89	90	94	84	10	709	0 / 6
6	284	562	102	310	71	33	288	6
7	89	970	94	124	321	9	13	3
8	90	970	94	124	321	9	13	3
9	94	970	94	124	321	9	13	3

Return to Home Page

If you would like to start at some point other than the beginning of the file set, you can select the file you want to begin with, then select the row within that file to begin with. After that, click the **Start Program** button. The MR72 will start playing from that row in that frequency file. This allows you to pick a previous session back up if you were unable to finish it. For example, in the screenshot above, the **Start Program** button was clicked and the play began with the first row of the fourth file.

Magnetic Frequency File Bank

When you select this function, the magnetic frequency file bank is displayed.

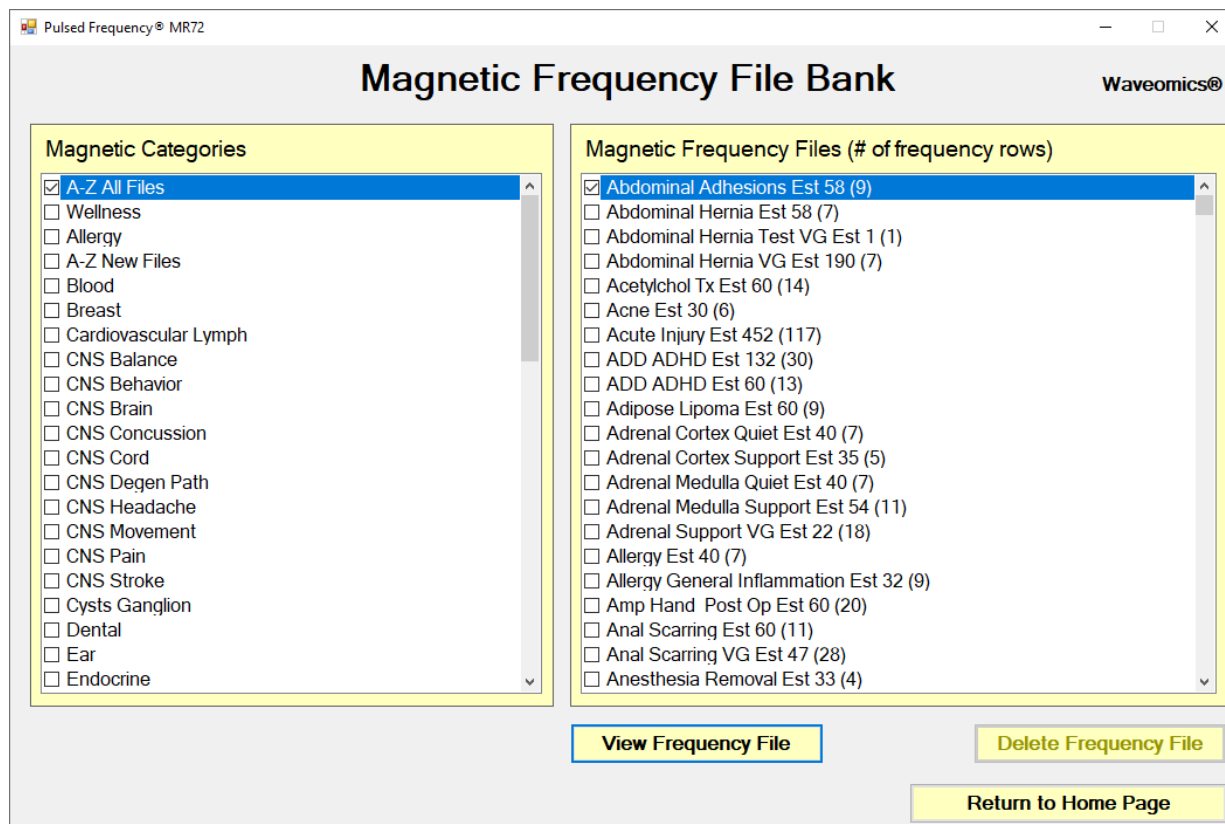

Frequency files are organized by category in the file bank. Files that have " Est " in the file name are established files that are provided with the software and cannot be overwritten or deleted. If you create your own frequency files, they cannot be saved with " Est " in the file name.

The **A-Z All Files** category is an alphabetical listing of all files in all categories in the file bank.

From this screen, you can view a frequency file or delete a frequency file. However, you will only be able to delete frequency files that you have created. Established (Est) files can never be deleted.

When you select a frequency file from one of the categories, and then click the **View Frequency File** button, you will be taken to another screen that will show all the frequencies in that file.

Pulsed Frequency® MR72

View Magnetic Frequency File

Waveomics®

Frequency File Name	Concussion Brief Est
Total Treatment Time	10
Category	CNS Concussion

Line #	CH 1	CH 2	CH 3	CH 4	CH 5	CH 6	CH 7	Time
1	396	396	417	528	639	741	852	2
2	321	94	970	9	970	200	1	2
3	94	200	94	310	9	94	1	2
4	49	94	310	49	81	310	1	2
5	6.8	38	35	102	6.8	38	1	2

Load Tissue/Function Analysis
Return to Magnetic Frequency File Bank
Return to Home Page

This screen shows all the frequencies that are programmed into the selected frequency file.

In order to see the Van Gelder Function/Condition and Structure/Tissue info for a specific frequency, right-click the frequency and a tooltip will be displayed with that information.

	Line #	CH 1	CH 2	CH 3	CH 4
	1	396	396	417	528
	2	321	94	970	9
▶	3	94	200	94	310
	4	49			49
	5	6.8	38	35	102

VGC Concussion, Nerve trauma, sexual power
 VGT Medulla, reticular activating system-RAS

When you have finished viewing the file, you can click **Return to Magnetic Frequency File Bank** to go back to the file bank and select another file.

Click **Return to Home Page** to be taken back to the main menu.

If you click the **Load Tissue/Function Analysis** button, the Magnetic Frequency File Components screen will appear.

Pulsed Frequency® MR72

Magnetic Frequency File Components

Waveomics®

Frequency File Name	Concussion Brief Est 10
Category	CNS Concussion

Magnetic Frequency File

Line #	1	2	3	4	5	6	7	Time
1	396	396	417	528	639	741	852	2
2	321	94	970	9	970	200	1	2
3	94	200	94	310	9	94	1	2
4	49	94	310	49	81	310	1	2
5	6.8	38	35	102	6.8	38	1	2

Function/Condition and Structure/Tissue Components of Frequency File

Descriptions in Red show Secondary Frequency

Alphabetical
Frequency
Occurrences

Van Gelder Function/Condition

Frequency Occurrences

Van Gelder Structure/Tissue

Frequency Occurrences

[Return to Spreadsheet](#)

At the top of the page, the spreadsheet for the selected frequency file is shown.

In order to see the Van Gelder Function/Condition and Structure/Tissue info for a specific frequency, right-click the frequency and a tooltip will be displayed with that information.

	Line #	CH 1	CH 2	CH 3	CH 4
	1	396	396	417	528
	2	321	94	970	9
▶	3	94	200	94	310
	4	49	VGC Concussion, Nerve trauma, sexual power VGT Medulla, reticular activating system-RAS		49
	5	6.8	38	35	102

When you scroll to the bottom of the page, the Function/Condition and Structure/Tissue Components for the file are shown.

Pulsed Frequency® MR72

Magnetic Frequency File Components

Waveomics®

Frequency File Name: Concussion Brief Est 10

Category: CNS Concussion

Highlighted in red above
Secondary Frequency

Alphabetical Frequency Occurrences

Van Gelder Function/Condition	Frequency	Occurrences
Poison Ivy	1	4
Allergic reaction, coryza	9	2
Copper, diabetes, balance chakra	35	1
Flu toxins-digestive, influenza-digestive	38	1
Vitality*, stop mitosis, *prolong cell life*	49	1
Secretions* to induce production of*-	81	1
Concussion, Nerve trauma, sexual power	94	3
Pyogenic infection-pus, staphylococcus	102	1
Paralysis 'reboot', anemia (pernicious), multiple sclerosis, strep-beta hemolytic-hemolyticus	321	1
Emotional component, balance	970	1

Van Gelder Structure/Tissue	Frequency	Occurrences
Brain (body) matrix	1	4
Pancreas	9	2
Liver	35	1
Gallbladder	38	1
Shoulder	81	1
Medulla, reticular activating system-RAS	94	3
Pineal	102	1
Solar nerve plexus	200	2
Anterior pituitary	310	2
Nerves	396	1
Consciousness, Limbic system	970	1

Return to SpreadSheet

The Van Gelder Function/Condition Analysis is shown in the spreadsheet on the left.

The Van Gelder Tissue/Structure Analysis is shown in the spreadsheet on the right.

Function/Conditions and Tissue/Structures highlighted in Red indicate Secondary Frequencies.

Click **Return to SpreadSheet** to return to the previous screen.

Create Magnetic Frequency File

If you would like to create your own frequency files, click the **Create Magnetic Frequency File** button from the main menu page.

Create Magnetic Frequency File

Categories

- ☐ A-Z All Files
- ☐ Wellness
- ☐ Allergy
- ☐ Blood
- ☐ Breast
- ☐ Cardiovascular Lymph

Frequency File Name:

Total Treatment Time:

Category:

Add Row

Line #	CH 1	CH 2	CH 3	CH 4	CH 5	CH 6	CH 7	Time	Delete
1									X

Save File **Open Van Gelder List** **Return to Home Page**

The page opens with a blank row. You can add a new row by clicking the **Add Row** button.

Create Magnetic Frequency File

Categories

- ☐ A-Z All Files
- ☐ Wellness
- ☐ Allergy
- ☐ Blood
- ☐ Breast
- ☐ Cardiovascular Lymph

Frequency File Name:

Total Treatment Time:

Category:

Add Row

Line #	CH 1	CH 2	CH 3	CH 4	CH 5	CH 6	CH 7	Time	Delete
1	111	222	333	444	555	666	777	10	X
2	987	666	340	1212	76	3	727	5	X

Save File **Open Van Gelder List** **Return to Home Page**

Frequencies in the range of 0.1 Hz to 5000 Hz can be added to the spreadsheet. You may add up to seven channels of frequencies. You must also add a time value in whole minutes.

Create Magnetic Frequency File

Categories

- ☐ Gout
- ☐ Immune Autoimmune
- ☐ Immune Support
- ☐ Infection
- ☒ John
- ☐ Kidney

Frequency File Name

Test

Total Treatment Time

15

Category

John

Add Row

Line #	CH 1	CH 2	CH 3	CH 4	CH 5	CH 6	CH 7	Time	Delete
1	111	222					777	10	X
2	987	666					727	5	X

The file "Test 15" has been saved in the "John" category.

OK

Save File

Open Van Gelder List

Return to Home Page


In order to see the Van Gelder Function/Condition and Structure/Tissue info for a specific frequency, right-click the frequency and a tooltip will be displayed with the information.

	Line #	CH 1	CH 2	CH 3	CH 4
	1	396	396	417	528
	2	321	94	970	9
	3	94	200	94	310
	4	49	VGC Concussion, Nerve trauma, sexual power VGT Medulla, reticular activating system-RAS		49
	5	6.8	38	35	102


To delete a row, just click the **X** button at the end of the row.

When you have finished creating the file, select a category to save it to. Also, give the frequency file a name. The name must not have " Est " in the file name. Once you have finished, click the **Save File** button and a message will be displayed indicating the file has been saved to the desired category.

If you have Microsoft Word installed, you can click the **Open Van Gelder List** button and the following dialog box will be displayed.

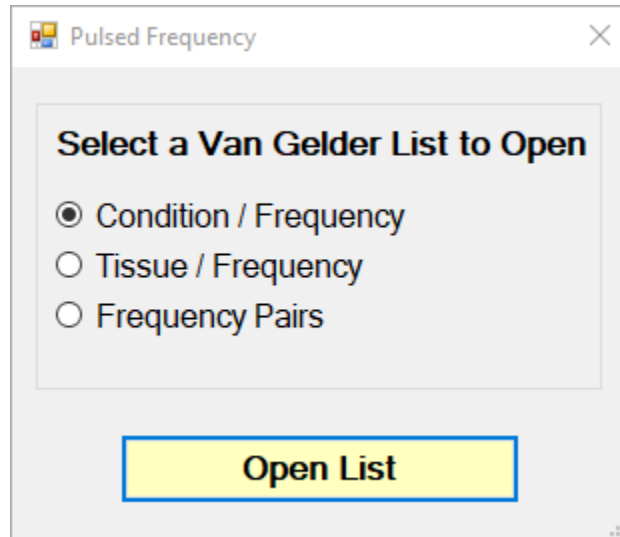

There are three different lists to choose from. After selecting one, click the **Open List** button. When you do, the list will open and your desktop will be organized in the following way.

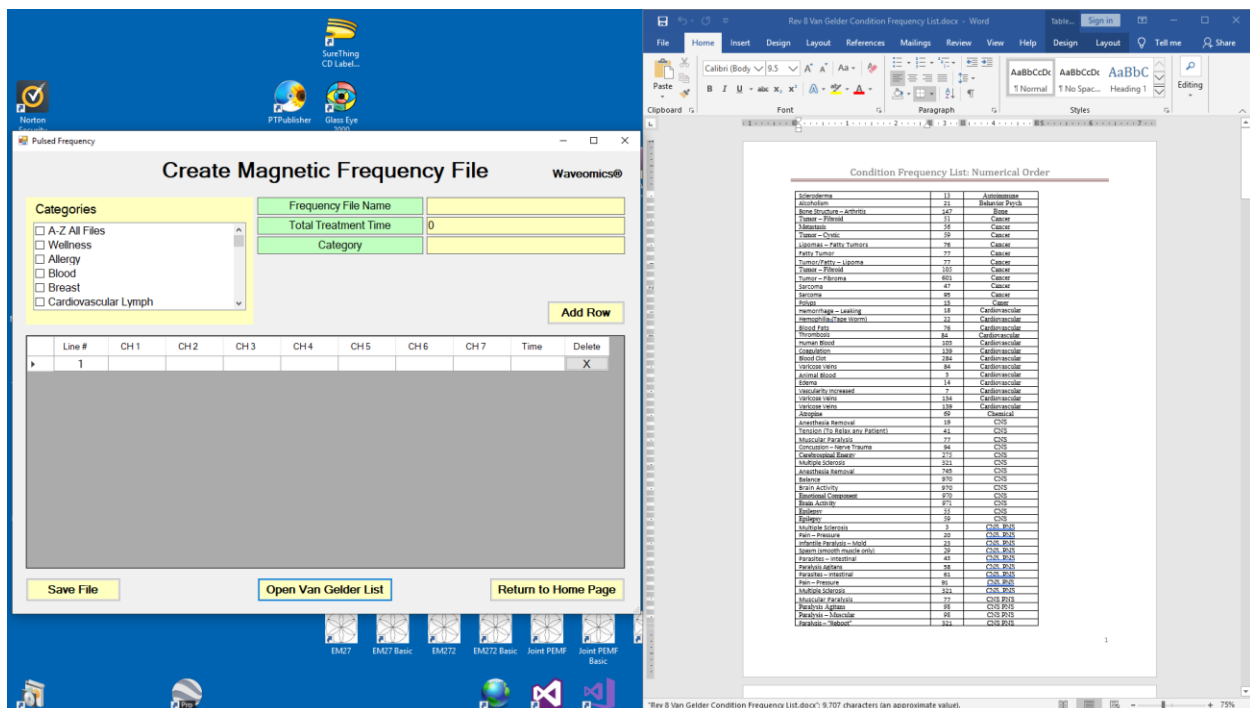

This layout allows you to refer to the list while creating the spreadsheet.

Edit Magnetic Frequency File

To edit an existing frequency file, click the **Edit Magnetic Frequency File** button from the main menu page. When you do this, the Magnetic Frequency File Bank will be displayed.

Magnetic Frequency File Bank

Magnetic Categories

- ☐ A-Z All Files
- ☐ Wellness
- ☐ Allergy
- ☐ Blood
- ☐ Breast
- ☐ Cardiovascular Lymph
- ☐ CNS Balance
- ☐ CNS Behavior
- ☐ CNS Brain
- ☐ CNS Concussion
- ☐ CNS Cord
- ☐ CNS Degen Path
- ☒ **CNS Headache**
- ☐ CNS Movement
- ☐ CNS Pain
- ☐ CNS Stroke
- ☐ Cysts Ganglion
- ☐ Dental
- ☐ Ear
- ☐ Endocrine
- ☐ Exercise

Magnetic Frequency Files (# of frequency rows)

- ☐ Headache Migraine Vascular Est 36 (6)
- ☒ **Headache Tension Est 40 (10)**

On this page, select a category and file, then click the **Edit Frequency File** button.

Edit Magnetic Frequency File SpreadSheet

Categories

- ☐ A-Z All Files
- ☐ Wellness
- ☐ Allergy
- ☐ Blood
- ☐ Breast
- ☐ Cardiovascular Lymph


Line #	CH 1	CH 2	CH 3	CH 4	CH 5	CH 6	CH 7	Time	Delete
1	200.0	94.0	970.0	124.0	321.0	9.0	49.0	4	X
2	7.8	396.0	417.0	528.0	639.0	741.0	852.0	4	X
3	13.0	443.0	124.0	100.0	13.0	443.0	13.0	4	X
4	13.0	443.0	77.0	396.0	443.0	77.0	396.0	4	X
5	40.0	157.0	77.0	100.0	142.0	480.0	783.0	4	X
6	284.0	157.0	77.0	100.0	142.0	480.0	783.0	4	X
7	13.0	480.0	396.0	142.0	480.0	396.0	142.0	4	X
8	970.0	562.0	27.0	23.0	35.0	38.0	37.0	4	X
9	970.0	13.0	355.0	33.0	102.0	35.0	7.8	4	X
10	49.0	443.0	124.0	77.0	33.0	35.0	33.0	4	X

The Edit Magnetic Frequency File SpreadSheet page will open for the selected file.

In order to see the Van Gelder Function/Condition and Structure/Tissue info for a specific frequency, right-click the frequency and a tooltip will be displayed with that information.

	Line #	CH 1	CH 2	CH 3	CH 4	
	1	396	396	417	528	
	2	321	94	970	9	
▶	3	94	200	94	310	
	4	49	VGC Concussion, Nerve trauma, sexual power VGT Medulla, reticular activating system-RAS			49
	5	6.8	38	35	102	

Make any changes you wish, then click the **Save File** button to save the changes. Remember, you cannot have an " Est " in the file name. If you do, you will get an error message like the one shown below.

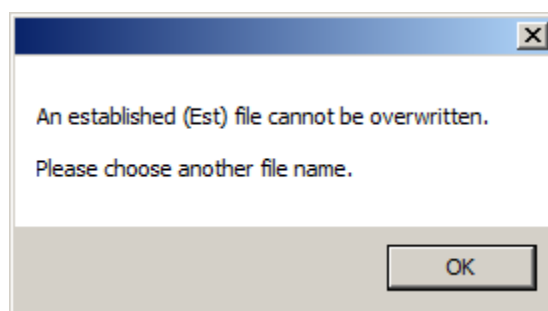

If you do have Est in the file name, just remove it, then click **Save File** again.

Edit Magnetic Frequency File SpreadSheet

Categories

- ☐ Immune Support
- ☐ Infection
- ☒ John
- ☐ Kidney
- ☐ Liver
- ☐ Miasm

Frequency File Name: Headache Tension

Total Treatment Time: 48

Category: John

Add Row


Line #	CH 1	CH 2	CH 3	CH 4	CH 5	CH 6	CH 7	Time	Delete
1	200.0	94					49.0	4	X
2	7.8	396					852.0	4	X
3	13.0	443					13.0	4	X
4	13.0	443					396.0	4	X
5	40.0	157					783.0	4	X
6	284.0	157.0	77.0	100.0	142.0	480.0	783.0	4	X
7	13.0	480.0	396.0	142.0	480.0	396.0	142.0	4	X
8	970.0	562.0	27.0	23.0	35.0	38.0	37.0	4	X
9	970.0	13.0	355.0	33.0	102.0	35.0	7.8	4	X
10	49.0	443.0	124.0	77.0	33.0	35.0	33.0	4	X
11	40.0	157.0	77.0	100.0	142.0	480.0	783.0	8	X

The file "Headache Tension 48" has been saved in the "John" category.


Save File **Open Van Gelder List** **Return to Home Page**

When the file has been saved, you will see a confirmation message giving you the name of the frequency file and the category it was saved to.

If you have Microsoft Word installed, you can click the **Open Van Gelder List** button and the following dialog box will be displayed.

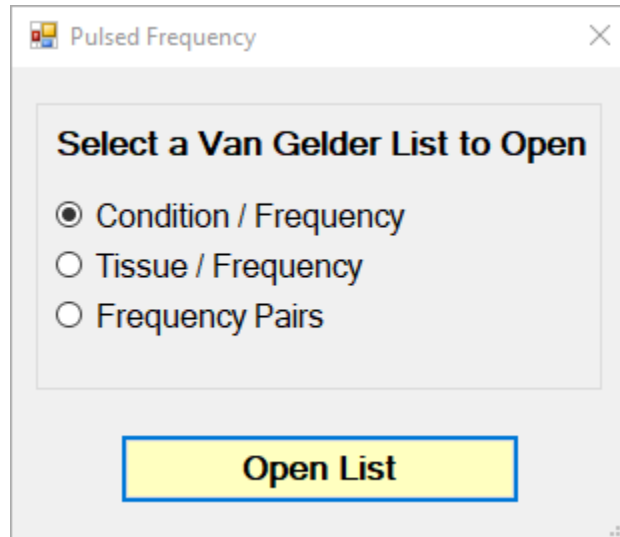

There are three different lists to choose from. After selecting one, click the **Open List** button. When you do, the list will open and your desktop will be organized in the following way.

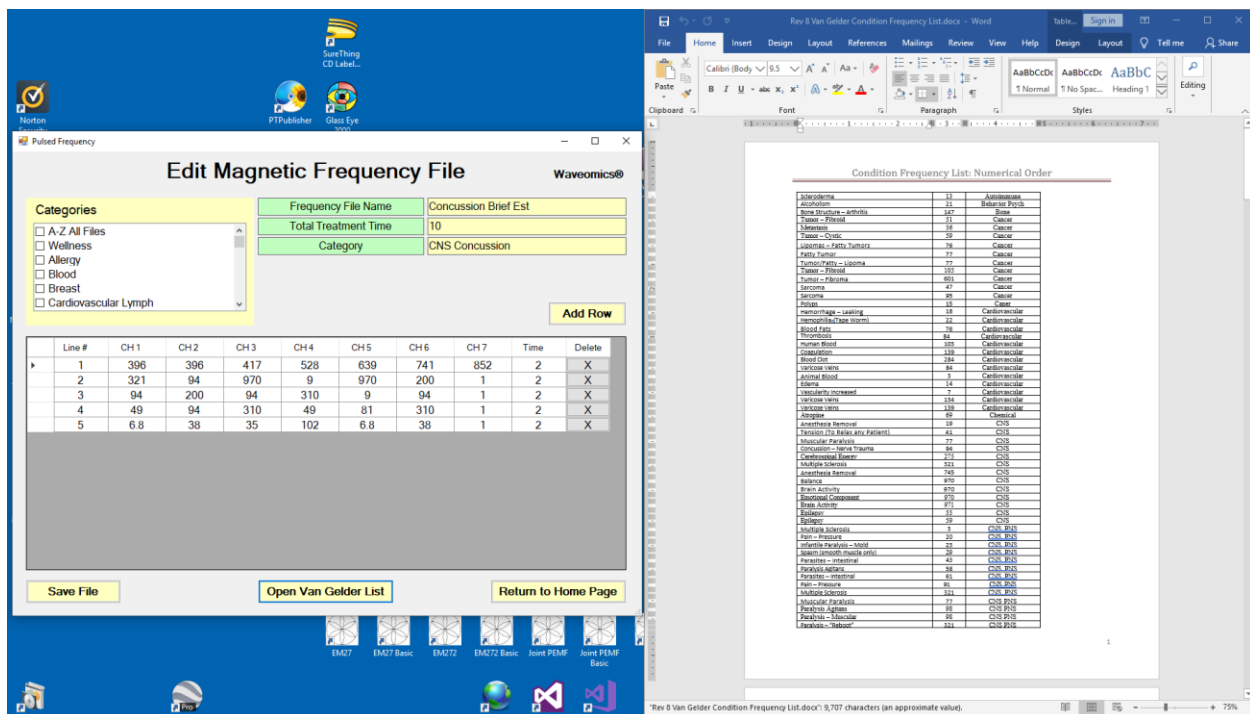


This layout allows you to refer to the list while creating the spreadsheet.

Create Play Magnetic Frequency File

The **Create Play Magnetic Frequency File** function allows you to create a new frequency file and play one row at a time. This is useful for testing the effect of different combinations of frequencies.

When you click the button on the main menu page, you are presented with this dialog box.

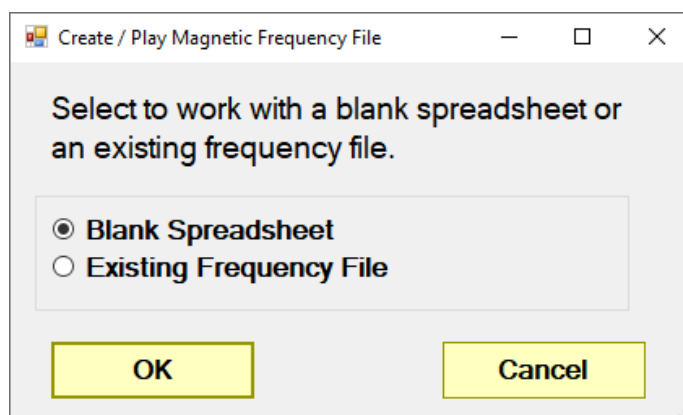

You can choose to work with a blank spreadsheet or an existing frequency file. If you choose to work with a blank spreadsheet, you would see the screen below.

Line #	CH1	CH2	CH3	CH4	CH5	CH6	CH7	Time	Play	Delete
1	111	222	333	444	555	666	777	5	Start	X

To begin, just click the **Add Row** button and add frequencies and a time value to the row. Then click the **Start** button. The **MR72™** will then output those frequencies for the specified amount of time.

Pulsed Frequency® MR72 v2.98 - Administrator

Create Play Frequency File

Waveomics®

Categories

- ☐ A-Z All Files
- ☐ Hidden Files
- ☐ New Trials
- ☐ Wellness
- ☐ Allergy
- ☐ Blood

Frequency File Name

Total Treatment Time: 5

Category

Add Row

Line #	CH 1	CH 2	CH 3	CH 4	CH 5	CH 6	CH 7	Time	Play	Delete
1	111	222	333	444	555	666	777	1 / 5	Stop	X

Save File Open Van Gelder List Return to Home Page

The **MR72™** will then output those frequencies for the specified amount of time and then stop. You can also press **Stop** at any time to stop the play.

Pulsed Frequency® MR72 v2.98 - Administrator

Create Play Frequency File

Waveomics®

Categories

- ☐ Skin
- ☐ Sleep
- ☐ Spinal Cord Injury
- ☐ Surgery
- ☒ Test
- ☐ Thyroid

Frequency File Name: A Test

Total Treatment Time: 5

Category: Test

Add Row

Line #	CH 1	CH 2	CH 3	CH 4	CH 5	CH 6	CH 7	Time	Play	Delete
1	111	222	333	444	555	666	777	5	Start	X

The file "A Test 5" has been saved in the "Test" category.

OK

Save File Open Van Gelder List Return to Home Page

If you would like to save the file, select a Category, enter a Frequency File Name, then click the **Save File** button.

If you chose to start with an existing frequency file, the Frequency File Bank dialog box will be displayed.

Frequency File Bank Waveomics®

Frequency File Categories

- ☒ A-Z All Files
- ☐ Wellness
- ☐ Allergy
- ☐ Blood
- ☐ Breast
- ☐ Cardiovascular Lymph
- ☐ CNS Balance
- ☐ CNS Behavior
- ☐ CNS Brain
- ☐ CNS Concussion
- ☐ CNS Cord
- ☐ CNS Degen Path
- ☐ CNS Headache
- ☐ CNS Movement
- ☐ CNS Pain
- ☐ CNS Stroke
- ☐ Cysts Ganglion
- ☐ Dental
- ☐ Ear
- ☐ Endocrine
- ☐ Exercise

Frequency Files

- ☒ Abdominal Adhesions Est 58 (9)
- ☐ Abdominal Hernia Est 58 (7)
- ☐ Acetylchol Tx Est 60 (14)
- ☐ Acne Est 30 (6)
- ☐ Acute Injury Est 452 (117)
- ☐ ADD ADHD Est 132 (30)
- ☐ ADD ADHD Est 60 (13)
- ☐ Adipose Lipoma Est 60 (9)
- ☐ Adrenal Cortex Quiet Est 40 (7)
- ☐ Adrenal Cortex Support Est 35 (5)
- ☐ Adrenal Medulla Quiet Est 40 (7)
- ☐ Adrenal Medulla Support Est 54 (11)
- ☐ Allergy Est 40 (7)
- ☐ Allergy General Inflammation Est 32 (9)
- ☐ Amp Hand Post Op Est 60 (20)
- ☐ Anal Scarring Est 60 (11)
- ☐ Anesthesia Removal Est 33 (4)
- ☐ Ankylosing Spondylitis Est 50 (11)
- ☐ Anxiety Est 30 (6)
- ☐ Appetite Suppression Est 60 (1)
- ☐ Arm Pain Emotional Est 54 (4)

Buttons: Create Category, Delete Category, Edit Frequency File, Delete Frequency File, Return to Home Page

Select a category and frequency file, then click Edit Frequency File button.

Create Play Frequency File Waveomics®

Categories

- ☒ A-Z All Files
- ☐ Hidden Files
- ☐ New Trials
- ☐ Wellness
- ☐ Allergy
- ☐ Blood

Frequency File Name: Concussion Brief Est

Total Treatment Time: 10

Category: CNS Concussion

Add Row

Line #	CH 1	CH 2	CH 3	CH 4	CH 5	CH 6	CH 7	Time	Play	Delete
1	396.0	396.0	417.0	528.0	639.0	741.0	852.0	2	Start	X
2	321.0	94.0	970.0	9.0	970.0	200.0	1.0	2	Start	X
3	94.0	200.0	94.0	310.0	9.0	94.0	1.0	2	Start	X
4	49.0	94.0	310.0	49.0	81.0	310.0	1.0	2	Start	X
5	6.8	38.0	35.0	102.0	6.8	38.0	1.0	2	Start	X

Buttons: Save File, Open Van Gelder List, Return to Home Page

After selecting a frequency file, it will be loaded and displayed in the above screen. From there, you can press the **Start** button on any row and play it for the specified amount of time, then it will stop.

Pulsed Frequency® MR72 v2.98 - Administrator

Create Play Frequency File

Waveomics®

Categories

- ☐ A-Z All Files
- ☐ Hidden Files
- ☐ New Trials
- ☐ Wellness
- ☐ Allergy
- ☐ Blood

Frequency File Name: Concussion Brief Est

Total Treatment Time: 10

Category: CNS Concussion

Add Row

Line #	CH1	CH2	CH3	CH4	CH5	CH6	CH7	Time	Play	Delete
1	396.0	396.0	417.0	528.0	639.0	741.0	852.0	2	Start	X
2	321.0	94.0	970.0	9.0	970.0	200.0	1.0	0 / 2	Stop	X
3	94.0	200.0	94.0	310.0	9.0	94.0	1.0	2	Start	X
4	49.0	94.0	310.0	49.0	81.0	310.0	1.0	2	Start	X
5	6.8	38.0	35.0	102.0	6.8	38.0	1.0	2	Start	X

Save File **Open Van Gelder List** **Return to Home Page**

You can also stop the play of the row at any time by pressing the **Stop** button.

Pulsed Frequency® MR72 v2.98 - Administrator

Create Play Frequency File

Waveomics®

Categories

- ☐ Skin
- ☐ Sleep
- ☐ Spinal Cord Injury
- ☐ Surgery
- ☒ **Test**
- ☐ Thyroid

Frequency File Name: Concussion

Total Treatment Time: 9

Category: Test

Add Row


Line #	CH1	CH2	CH3	CH4	CH5	CH6	CH7	Time	Play	Delete
1	396.0	396.0					52.0	2	Start	X
2	321.0	94.0					1.0	1	Start	X
3	94.0	200.0					1.0	2	Start	X
4	49.0	94.0					1.0	2	Start	X
5	6.8	38.0	35.0	102.0	6.8	38.0	1.0	2	Start	X

Save File **Open Van Gelder List** **Return to Home Page**


If you have made changes and would like to save the file, select a Category, enter a Frequency File Name, then click the **Save File** button.

Otherwise, click the **Return to Home Page** button to go back to the main menu. You will be asked if you want to save the file. If you do, click **Yes**. If you don't, click **No**, and the changes will be discarded.

If you have Microsoft Word installed, you can click the **Open Van Gelder List** button and the following dialog box will be displayed.

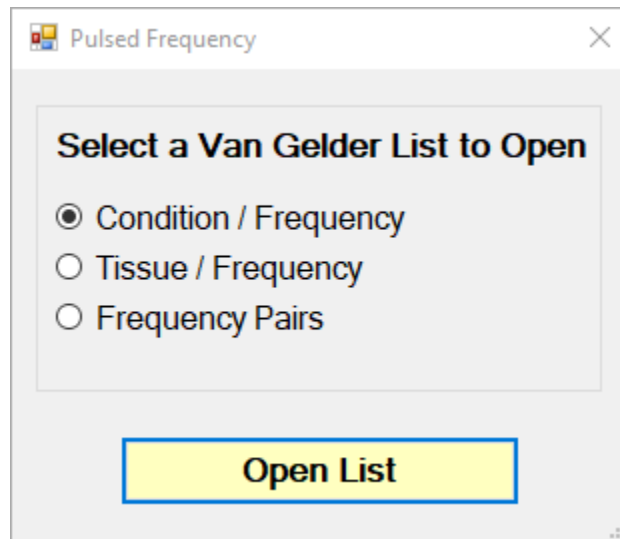

There are three different lists to choose from. After selecting one, click the **Open List** button. When you do, the list will open and your desktop will be organized in the following way.

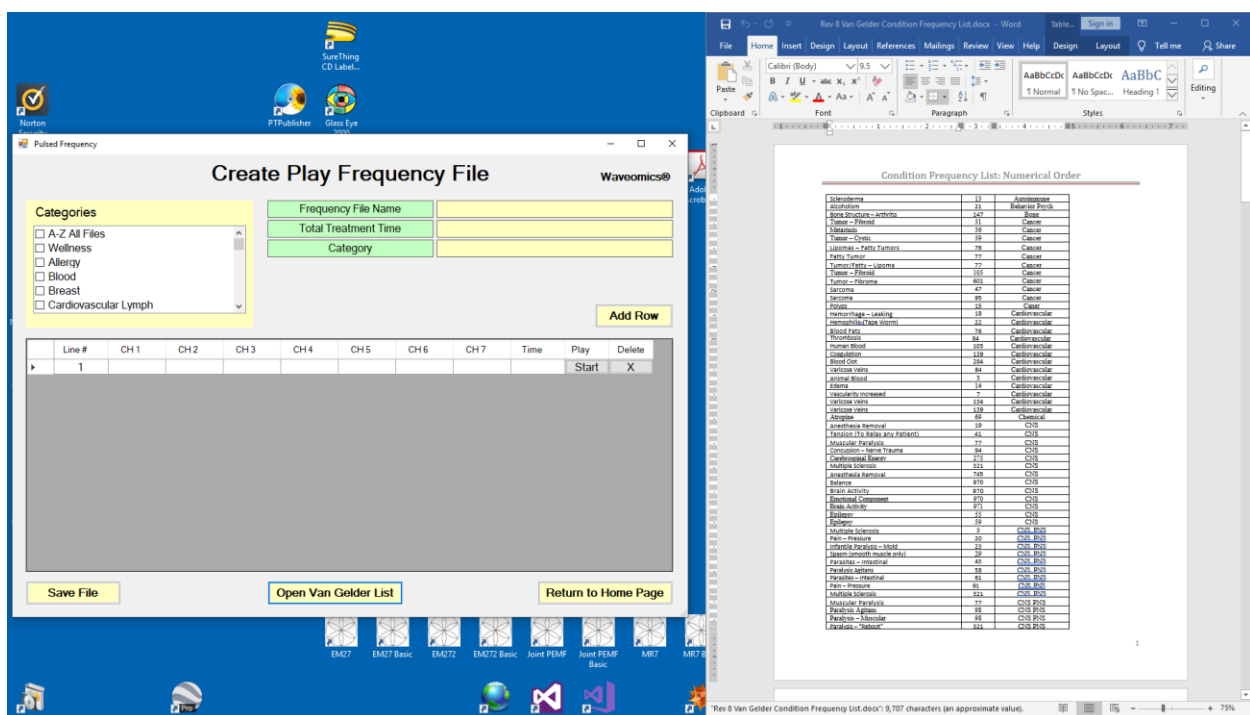

This layout allows you to refer to the list while creating the spreadsheet.

Treatment Files

When you click the **Treatment Files** button from the main menu page, the following screen will appear.

Treatment Files

Select Name: Doe, John
Unspecified,

Treatment Files for John Doe SN: 00010864

Local Machine Cloud Combined

	Date	Treatment	Magnetic Frequency Files
1	10/11/2018 19:06:26	Sleep 1 Est 587	Concussion Brief Est 10 Miasm General Est 9 Quiet Sympathetic Est 20 Sleep Natural Rhythm Est 458 Relax Balance Est 30 PTSD Stress Est 60
2	10/11/2018 19:05:22	Sleep Test 300	Sleep Quiet Balance Est 80 Sleep Quiet Sympathetic Est 220
3	10/11/2018 19:03:53	Trauma Acute 234	Soft Tissue Acute Est 32 Trauma Acute Est 152 Brain Trauma Concussion Est 50
4	10/11/2018 19:02:38	Pancreas 96	Pancreas Support Est 46 Pancreas Dysfunction Est 50
5	10/11/2018 19:01:22	Foot Est 293	Gout Acute Chronic Est 60 Periph Neuropathy Est 61 Periph Neurop Diabetic Est 62 Plantar Fasciitis Est 60 Plantar Fasciitis Bone Spur Est 50
6	10/11/2018 18:56:47	Concussion Est 210	Concussion Brief Est 10 CNS Forebrain Acute Est 30 Reset CNS Est 50 CNS Medulla Acute Est 30 Brain Fog Est 30

Add New Name Send Treatment to Magnetic Frequency Compiler Delete Row Print Preview Save to Text File
 Delete Name Download All Treatments Print Return to Home Page

The Treatment Files page is where you can look at the treatments that have been saved for each person. Just click the name of any person in the list, and their treatments will be loaded and displayed.

Just as in the Compiler, you can also add a new name to the list. To do this, click the **Add New Name** button and the following dialog box will appear.

Create New Name

Enter New Name

First Name Last Name

Enter Close

When you enter a First Name and Last Name and click the **Enter** button, the new name will be added to the list.

You can also delete a name from the list by selecting a name and then clicking the **Delete Name** button.

Treatment Files

Select Name Treatment Files for John Doe SN: 00010422

	Date	Treatment	Magnetic Frequency Files
1	10/11/2018 19:16:47	Sleep 1 Est 587	Concussion Brief Est 10 Miasm General Est 9 Quiet Sympathetic Est 20 Sleep Natural Rhythm Est 458 Relax Balance Est 30 PTSD Stress Est 60
2	10/11/2018 19:15:52	Sleep Test 300	Sleep Quiet Balance Est 80 Sleep Quiet Sympathetic Est 220
3	10/11/2018 19:14:52	Trauma Acute 234	Soft Tissue Acute Est 32 Trauma Acute Est 152 Brain Trauma Concussion Est 50
4	10/11/2018 19:14:01	Pancreas 96	Pancreas Support Est 46 Pancreas Dysfunction Est 50
5	10/11/2018 19:12:53	Foot Est 293	Gout Acute Chronic Est 60 Periph Neuropathy Est 61 Periph Neurop Diabetic Est 62 Plantar Fasciitis Est 60 Plantar Fasciitis Bone Spur Est 50
6	10/11/2018 19:11:58	Concussion Est 210 210	Concussion Brief Est 10 CNS Forebrain Acute Est 30 Reset CNS Est 50 CNS Medulla Acute Est 30 Brain Fog Est 30

One of the nice things about the Treatment Files function is that you can select any treatment and send it back to the Compiler. Just select a treatment, click the **Send Treatment to Magnetic Frequency Compiler** button, and you will be sent to the Compiler where that treatment will be loaded.

Pulsed Frequency

Compiler

Categories

- ☒ A-Z All Files
- ☐ A-Z Combined
- ☐ Commonly Used Compiled Files
- ☐ Wellness
- ☐ Allergy
- ☐ Blood
- ☐ Breast
- ☐ Cardiovascular Lymph
- ☐ CNS Balance
- ☐ CNS Behavior
- ☐ CNS Brain
- ☐ CNS Concussion
- ☐ CNS Cord
- ☐ CNS Degen Path
- ☐ CNS Headache
- ☐ CNS Movement
- ☐ CNS Pain
- ☐ CNS Stroke
- ☐ Cysts Ganglion
- ☐ Dental
- ☐ Ear
- ☐ Endocrine

Frequency Files (# of freq rows)

- ☐ Abdominal Adhesions Est 58 (9)
- ☐ Abdominal Hernia Est 58 (7)
- ☐ Acetylchol Tx Est 60 (14)
- ☐ Acne Est 30 (6)
- ☐ Acute Injury Est 452 (117)
- ☐ ADD ADHD Est 132 (30)
- ☐ ADD ADHD Est 60 (13)
- ☐ Adipose Lipoma Est 60 (9)
- ☐ Adrenal Cortex Quiet Est 40 (7)
- ☐ Adrenal Cortex Support Est 35 (5)
- ☐ Adrenal Medulla Quiet Est 40 (7)
- ☐ Adrenal Medulla Support Est 54 (11)
- ☐ Allergy Est 40 (7)
- ☐ Allergy General Inflammation Est 32 (9)
- ☐ Amp Hand Post Op Est 60 (20)
- ☐ Anal Scarring Est 60 (11)
- ☐ Anesthesia Removal Est 33 (4)
- ☐ Ankylosing Spondylitis Est 50 (11)
- ☐ Anxiety Est 30 (6)
- ☐ Arm Pain Emotional Est 54 (4)
- ☐ Asthma Adv Est 40 (9)
- ☐ Asthma Est 42 (8)

Compiled Frequency File Name

Number of Repeats (Max 255)


Play Order	Frequency File	Time	Delete
1	Gout Acute Chronic Est 60	60	X
2	Periph Neuropathy Est 61	61	X
3	Periph Neurop Diabetic Est 62	62	X
4	Plantar Fasciitis Est 60	60	X
5	Plantar Fasciitis Bone Spur Est 50	50	X

Total Number of Minutes (Max 999)

Total Number of Rows (Max 500)

With the treatment loaded into the Compiler, you can edit it or click the **Transfer Treatment to Device** button to transfer it to your MR72.


You can also delete any treatment from the treatment history of a specific person.

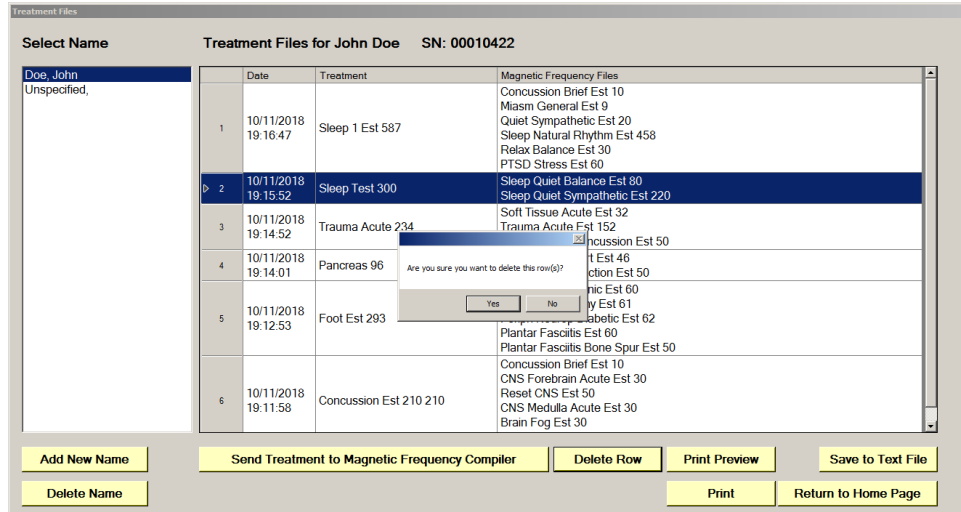

Select the treatment you want to delete and a confirmation dialog will be displayed where you can answer **Yes** or **No**. If you answer Yes, the treatment will be deleted.

To delete a person and their entire treatment history, click the **Delete Name** button. Be careful with this as once a person is deleted, they are gone permanently.


The Treatment Files function also has Print and Print Preview features. To preview something before printing, select the rows you want to print and click the Print Preview button.

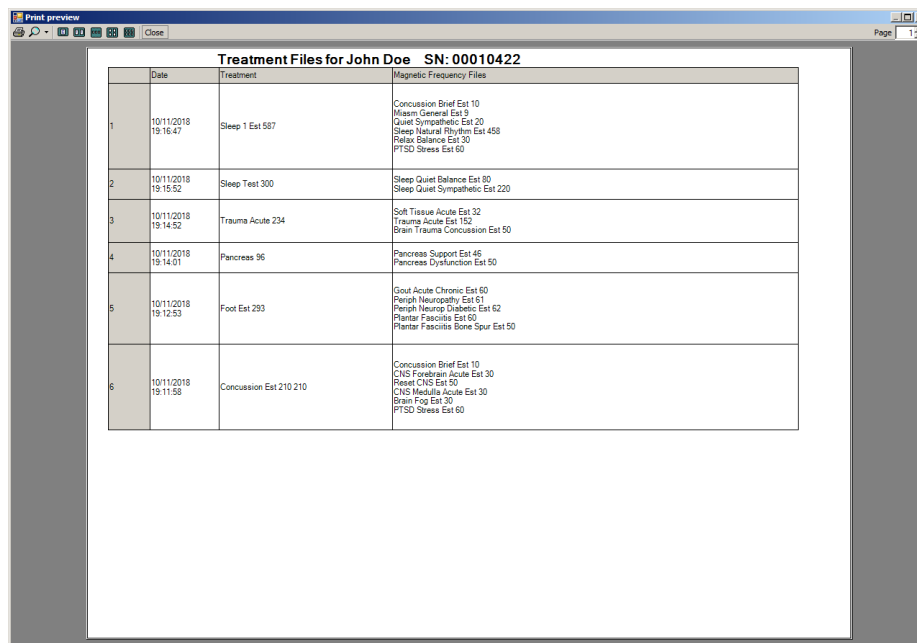

Once you are satisfied, you can click the Printer icon in the Print Preview window and your treatments will print.

If you don't want to preview, just select the treatments you want to print and then click the **Print** button.

The final capability in the Treatment Files section is **Save to Text File**. This function works similarly to **Print**, except when you select the treatments you want, then click the **Save to Text File** button, a dialog will open that allows you to save the treatments to a text file on your hard drive.

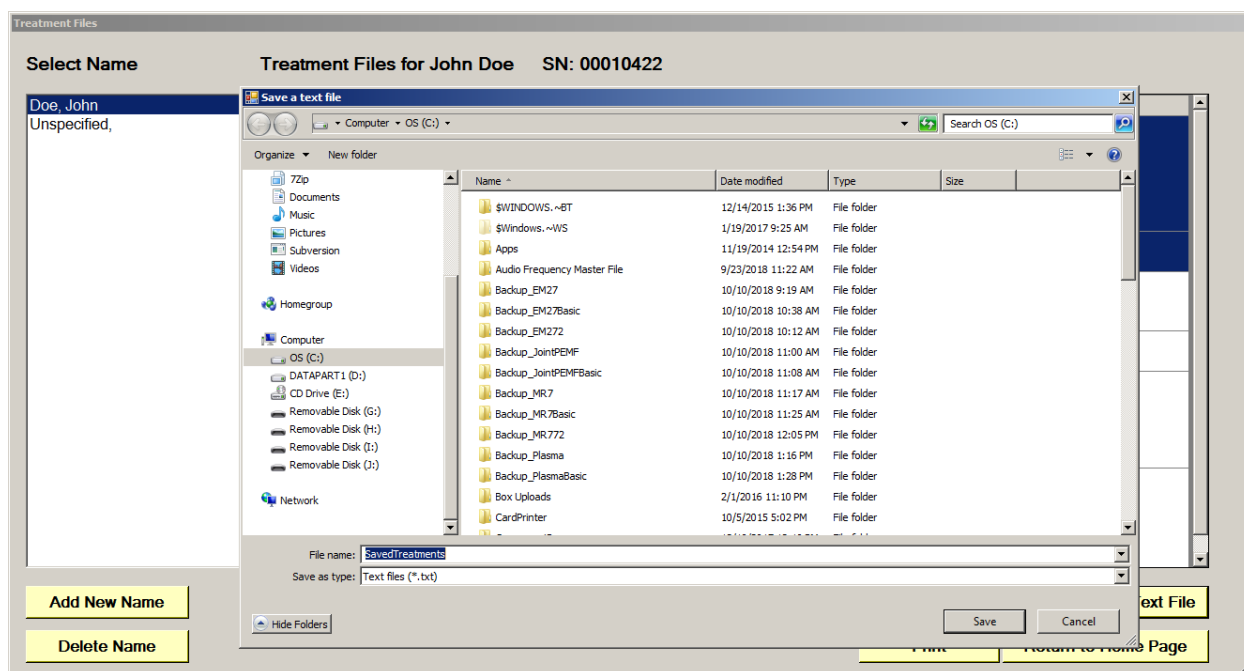


Select a location on your hard drive, enter a name for the text file, and click the **Save** button. The treatments will then be saved to that location.

File Storage

When the **File Storage** button is clicked on the main menu page, you will be presented with a dialog box that has the following tabbed pages.

- ☐ Backup / Restore
- ☐ Detect Method
- ☐ Serial Number

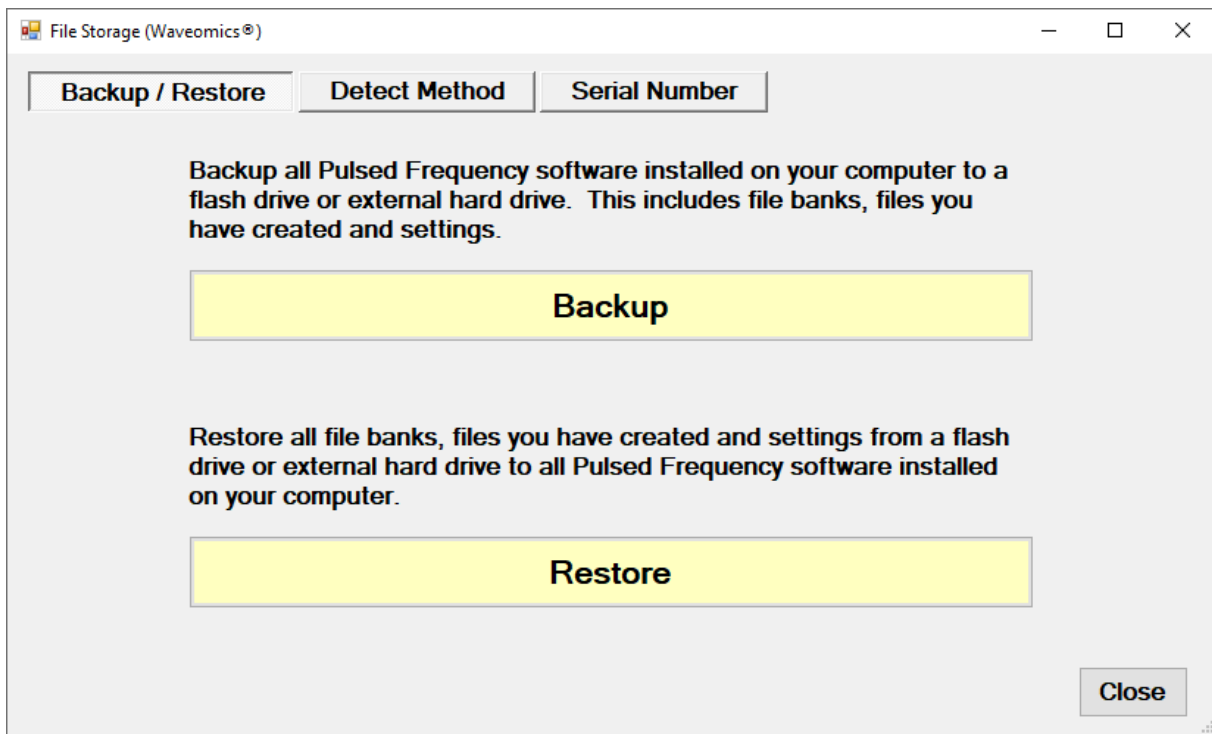


The **Backup / Restore** tab has functions which allow you to back up and restore your Pulsed Frequency software.

The **Backup** function will back up all the Pulsed Frequency software installed on your computer to a flash drive or external hard drive. This includes file banks, files you have created and your settings.


The **Restore** function restores all file banks, files you have created and settings from a flash drive or external hard drive to all the Pulsed Frequency software installed on your computer.

To use the **Backup** function, click the **Backup** button.

When you click **Backup**, the following dialog box will appear.

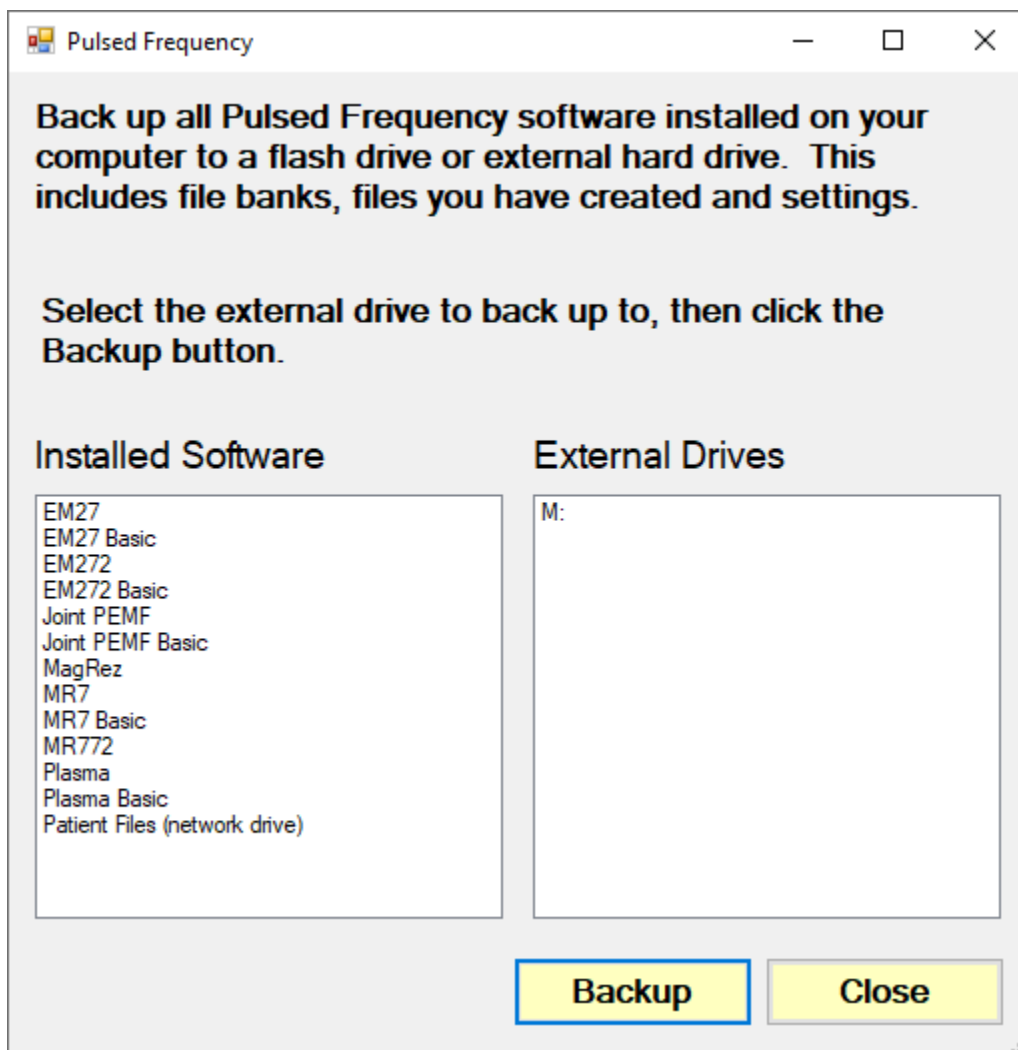


The Pulsed Frequency software installed on your computer is listed on the left. The external drives are listed on the right. Select an external drive from the list on the right, then click the **Backup** button.

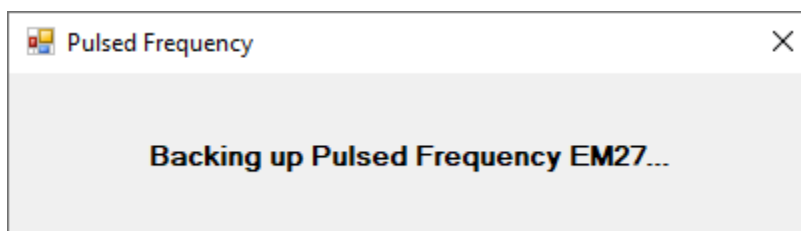


While the function is backing up all your software to the external drive, you will see messages displayed like the one above that show you what version is currently being backed up. When the process has finished, you will be returned to the **Backup / Restore** page.


To use the **Restore** function, click the **Restore** button.

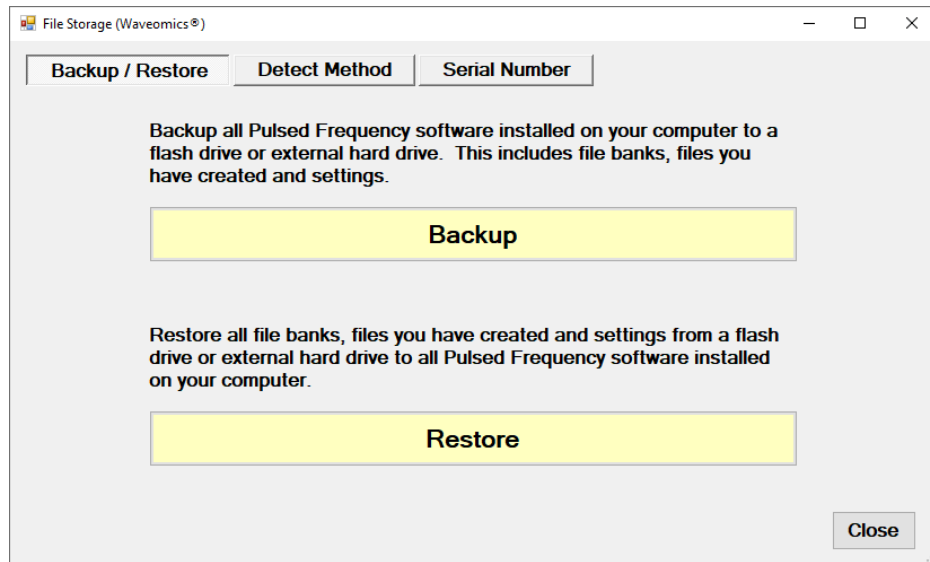

When you click **Restore**, the following dialog box will appear.

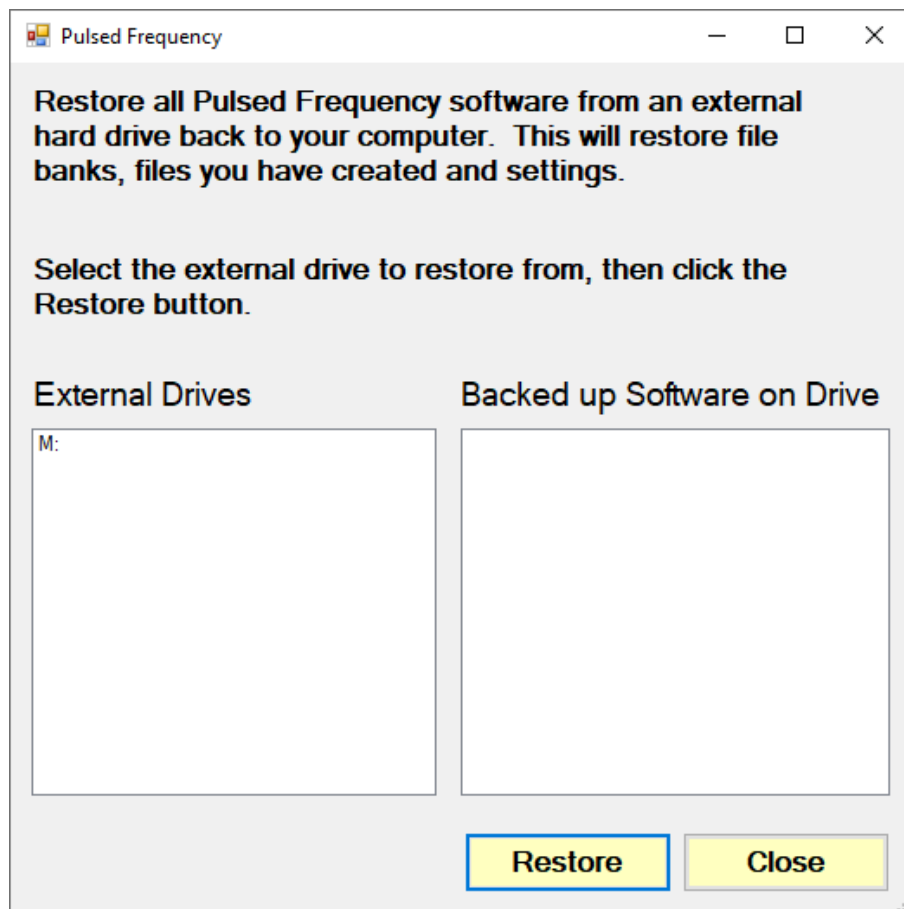

The list of external drives connected to your computer will be on the left. Select a drive.

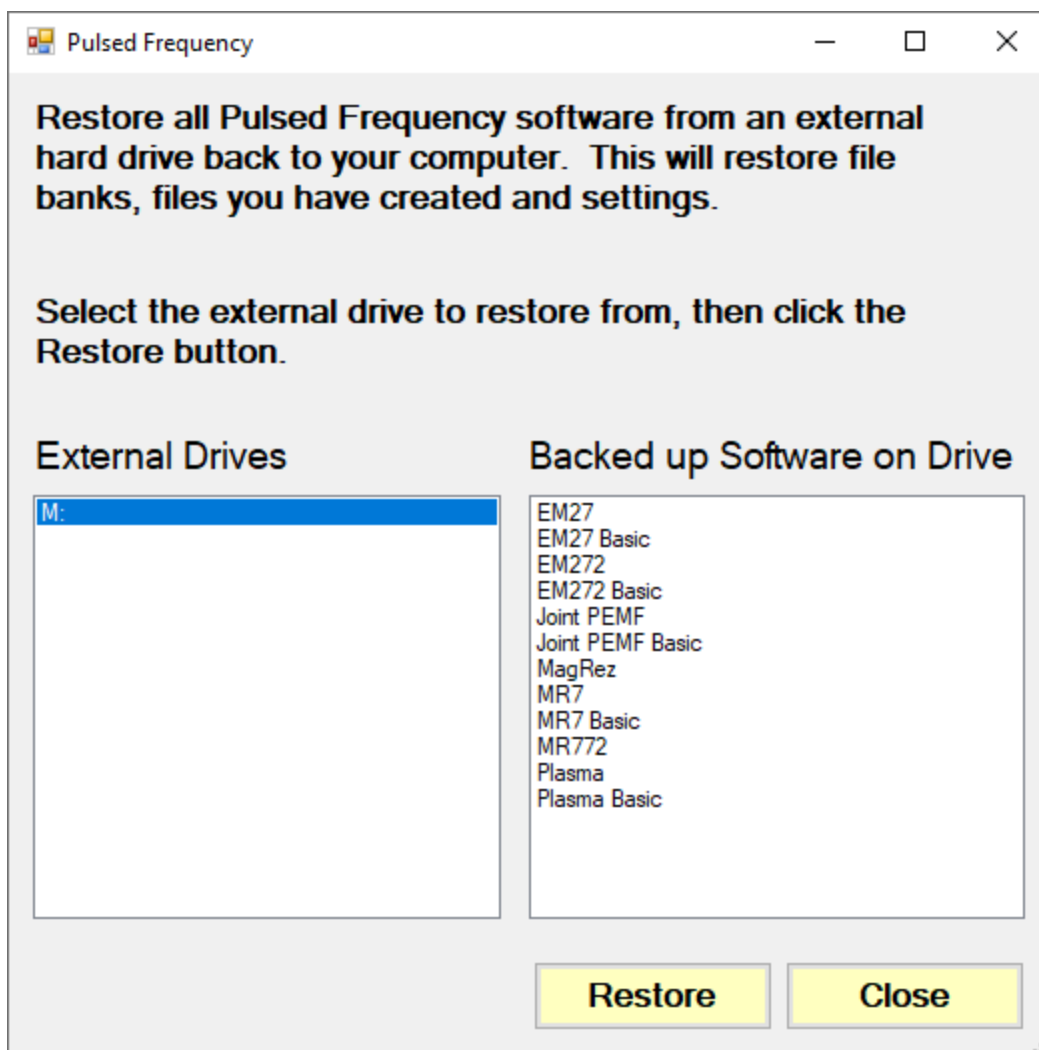


After you have selected an external drive, the list of software backed up on that drive will appear on the right. When you click Restore, the program will restore the files to only the software you have installed on the computer.


For example, let's say you want to back up your desktop computer and restore onto a laptop. You have all 12 versions of Pulsed Frequency software on the desktop computer and when you backed up to the external drive, all 12 versions were backed up. But the laptop you want to restore to only has 4 versions of Pulsed Frequency software. That is fine. The program will only restore the files to the 4 versions of software you have on the laptop computer.

If you are a practitioner and have a clinic with multiple rooms each having computers with Pulsed Frequency software installed, you should backup from the computer that has the most editions of the software installed. When you take the external drive to each of the other rooms, you can be assured that all the software on the computers in those rooms will be restored.

After you press the **Restore** button, the program will let you know what Pulsed Frequency software is currently being restored.

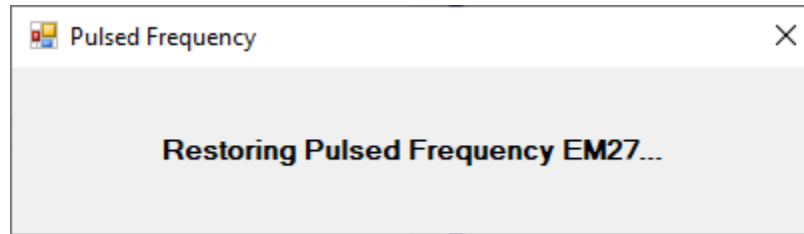

The above message will change as the files for each edition of the Pulsed Frequency software is restored.

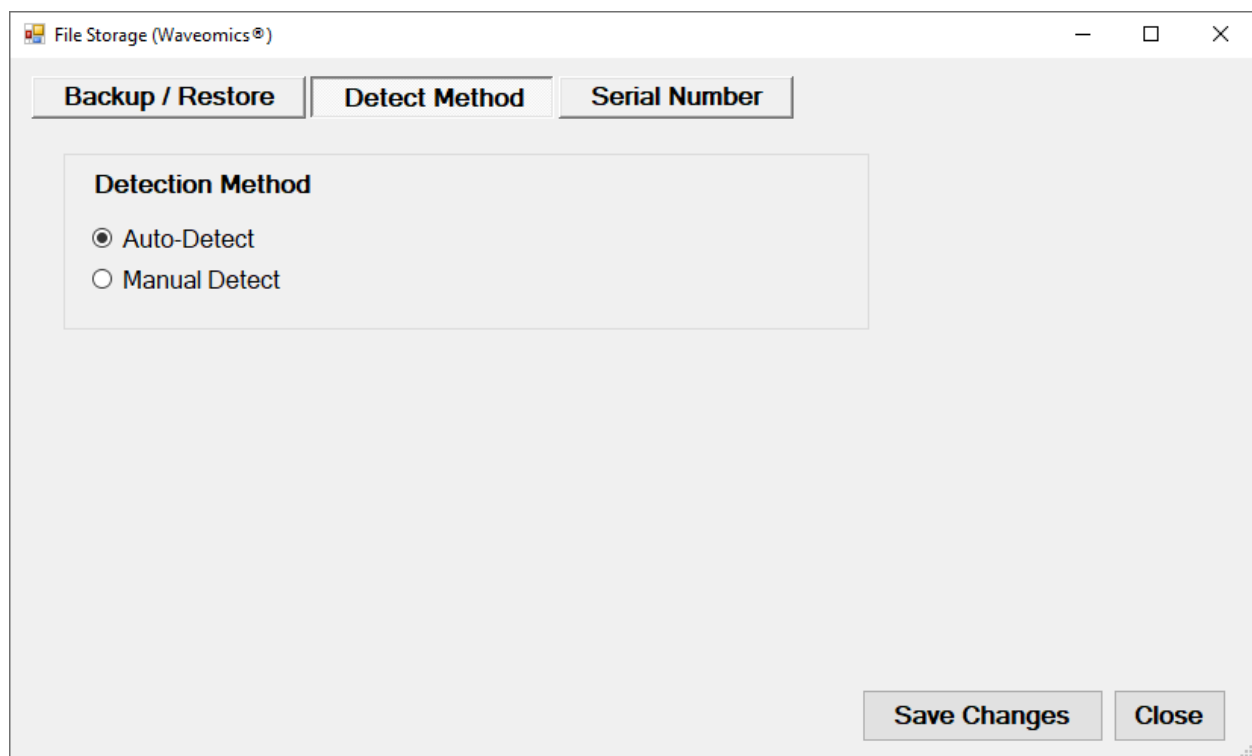


The **Detect Method** tab allows you to select the method of device detection. When the software is first installed, **Auto-Detect** is selected by default. This means that your **MR72** will be detected automatically when you connect it to the computer. In most cases, the software will work fine if you leave this setting alone.

If you change the Detect Method setting, click the **Save Changes** button to save your choice.


In a very small percentage of cases, the **Manual Detect** setting may work better. This is usually only needed on older computers that are slower. The only way to tell if you need to switch to **Manual Detect** is if your **MR72** has continuous problems being detected when Auto-Detect is selected.

To use Manual Detect, select the setting, click **Save Changes**, then click the **Close** button. On the main menu page, click **Close Program** to exit from the software.

To learn how to do manual detection, please go to the section of the manual entitled, **MR72 Manual Detection**.

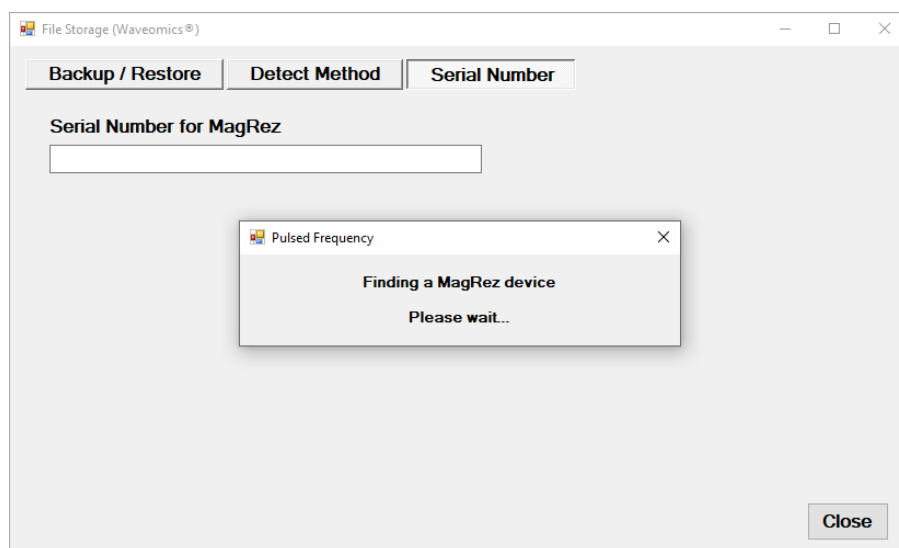

The **Serial Number** tab will display the serial number of your **MR72**, if it is connected to the computer. The software first looks for the **MR72** device(s).

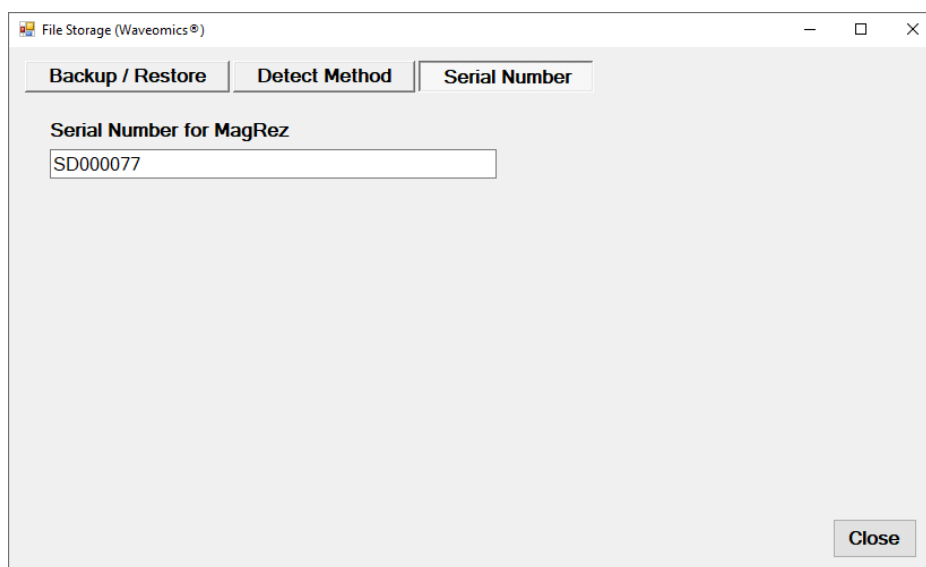

When you are finished with the **File Storage** function, just click the **Click** button.

Troubleshooting

If you have problems detecting your MR72 device, you will need to troubleshoot the problem. To do this, exit from the software and try the following solutions.

Solution 1

Even though you have the USB cable plugged into the MR72 and to the computer, you may not have a good connection. Unplug the cable from both the MR72 and the computer, then plug the cable back into both places. Next, run the software, click View Frequency Files in Device, and see if the words, "MR72 is not connected" still appear on the screen. If they don't, your problem is solved. You can now proceed to the Software User Guide section. If you still see the words, proceed to Solution 2.

Solution 2

The most common cause of a connection problem is that Windows cannot see your device. Try plugging the USB cable into a different USB port on your computer. Also, unplug the cable from your MR72 and plug it back in. Run the software again, click View Frequency Files in Device and see if you can see the files loaded into your MR72. If you can see the files, proceed to the Software User Guide section. If you still get the message, "MR72 is not connected", proceed to Solution 3.

Solution 3


If you are still having a problem, try plugging the larger end of the USB cable into a USB hub. The hub must be powered for this to work. A powered USB hub is where a power cable runs from the hub to an AC adapter that plugs into a wall outlet. With the MR72 plugged into the hub, run the software and try to load a treatment. If you can, your problem is solved.

Solution 4

Another cause of a connection problem is a bad USB cable. If you suspect your cable, then replace it and try again.

Solution 5


If all other solutions have failed, a final check is to run the Device Manager.

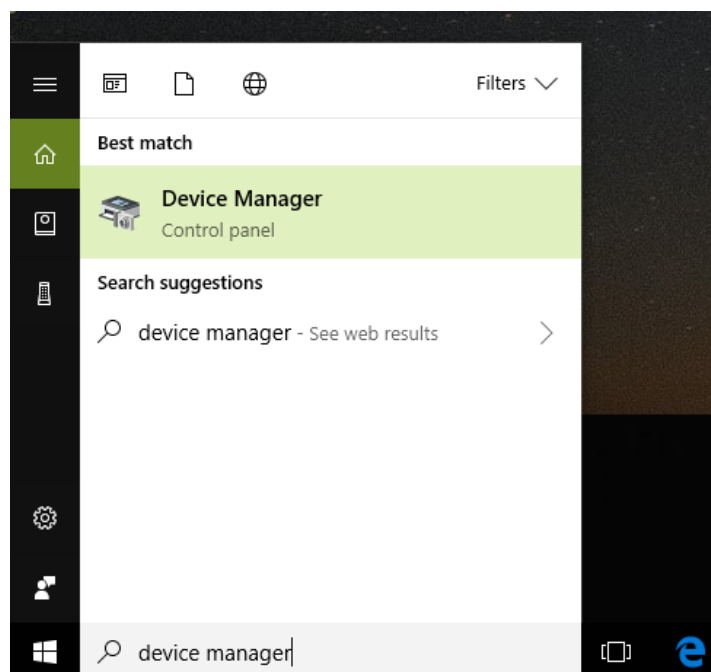

If you are using Windows 10, go to the lower left hand corner of the screen and enter the words "device manager". When that choice appears in the list, click on it.


If you are using Windows 8 or 8.1, click the flag in the lower left hand corner and type "device manager." When that choice appears in the list, click on it.

If you are on Windows 7, click the Start button in the lower left hand corner, and enter "device manger" in the search box. When that choice appears in the list, click on it.

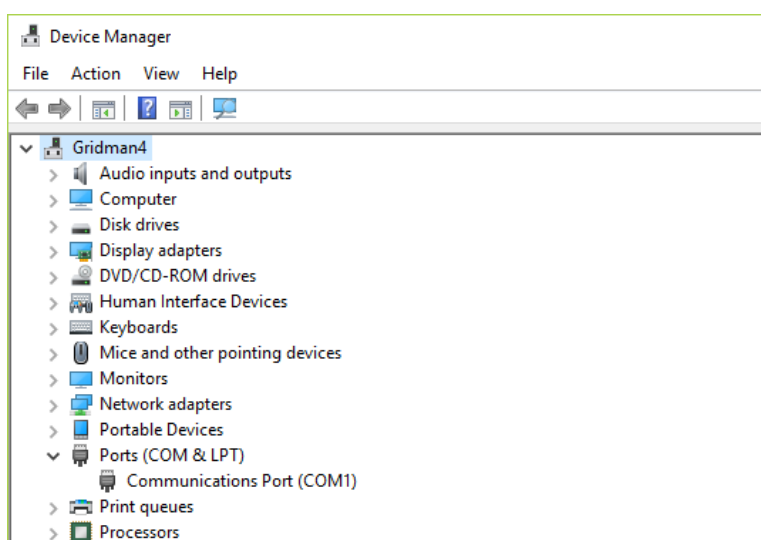

In Device Manager, click the arrow next to Ports (COM & LPT) in order to expand the list. If the MR72 is connected and you see something similar to the screenshot above, then Windows

cannot see your device. Try any of the above solutions then come back to Device Manager and look at the list.

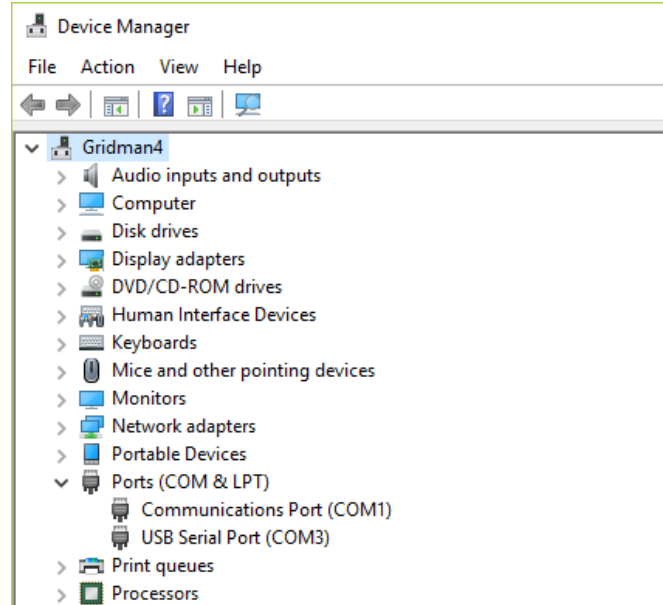

When Windows can see the MR72, you will see an entry similar to the one above that says, "USB Serial Port (COM3). It may show a different COM port, but that is okay. The main thing to remember is that when Windows can see your MR72, it will assign a COM port to it. You should now be able to run the software and transfer treatments to the MR72.

MR72 Manual Detection

Please follow these steps in order to manually detect your MR72.

On Windows 10, click the Windows flag in the lower left corner of the screen and scroll down the list of programs until you see the Pulsed Frequency folder. Expand that folder and select **Detect MR72**.


On Windows 8 or 8.1, click the Windows flag in the lower left corner of the screen, type "detect MR72" and when that item is displayed in the list on the right, select it to run the utility.

On Windows 7, go to the Start Menu, click All Programs, scroll down to the Pulsed Frequency folder and select the **Detect MR72** program. Make sure your MR72 is not connected to the computer when you do this.


After you have clicked on the shortcut, you will get a warning from Windows saying "Do you want to allow this app from an unknown publisher to make changes to your device?" Click "Yes". Follow the instructions on the screen to detect your device.




On the first page of the utility program, click the Detect Device button. The following dialog box will then be displayed.

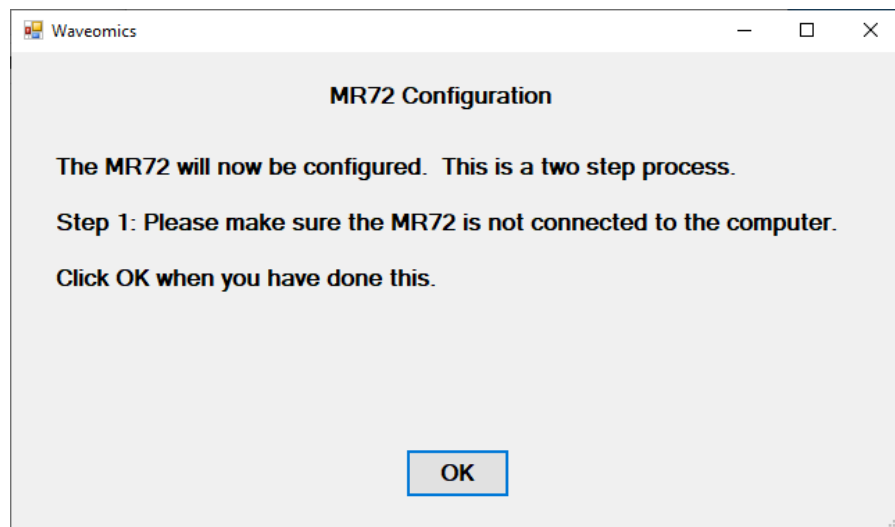


Make sure the MR72 is not connected to the computer, then click the **OK** button.

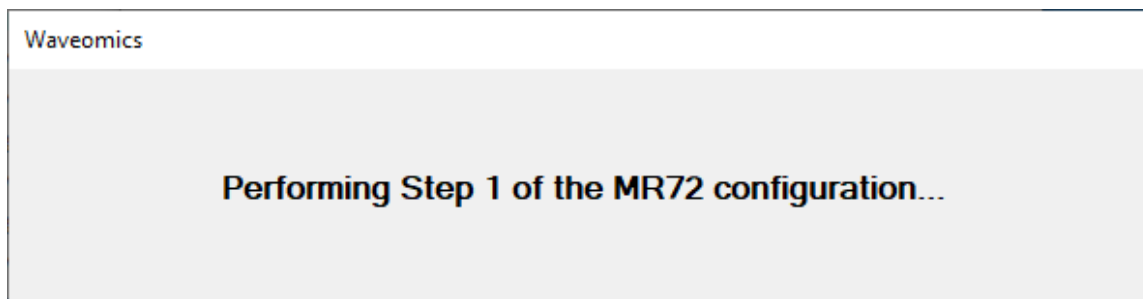

Here, the program is looking at your system without the MR72 connected. After it is finished, the following dialog box will be displayed.

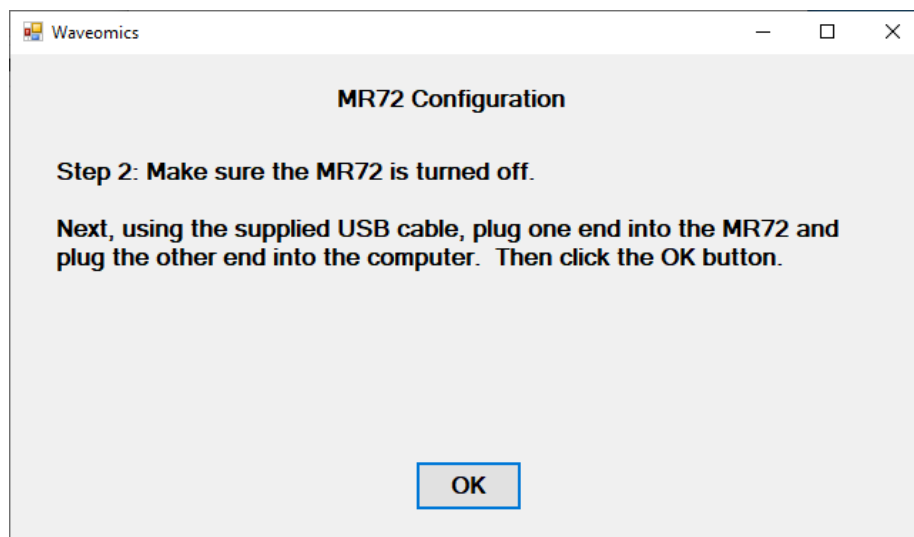


Make sure the MR72 is turned off, connect it to the computer, then click the **OK** button.

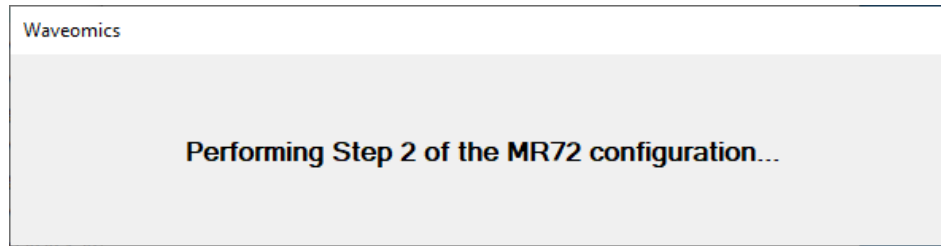

Here, the utility program is looking at your system with the MR72 connected.



When it has detected your device, you will be returned to the main screen of the program.

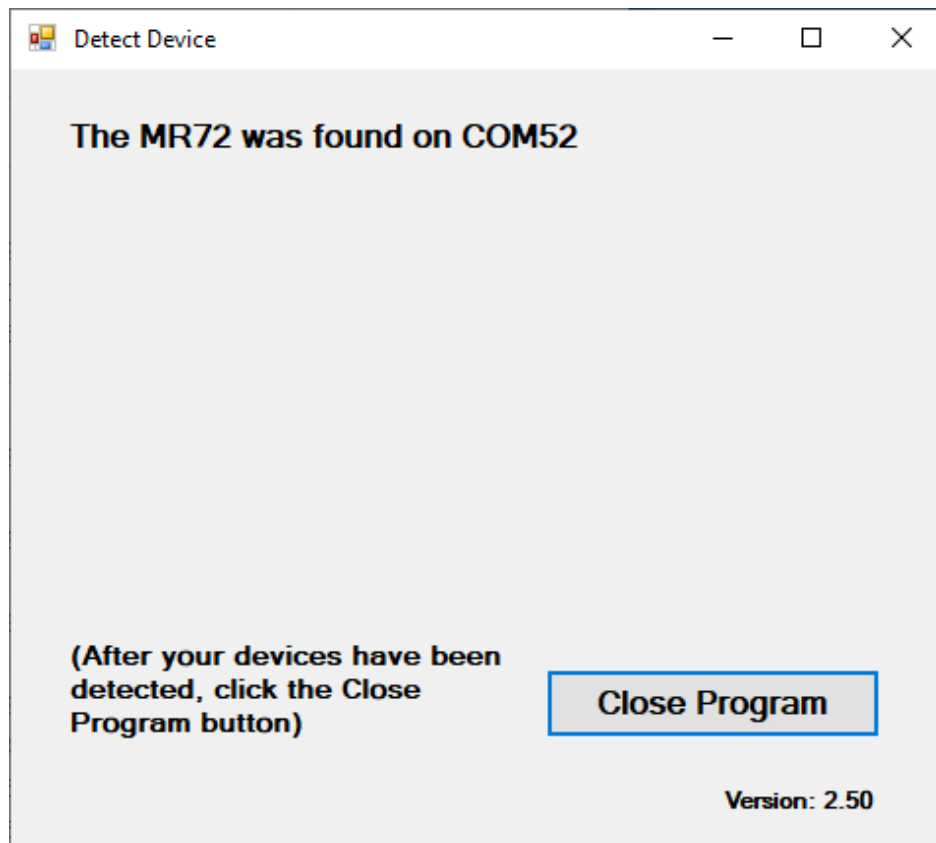

The location of the MR72 will be displayed on the screen and saved in the configuration information for the Pulsed Frequency MR72 software. You can now click the **Close Program** button to exit the program. This completes the manual detection process.

The Pulsed Frequency™ software can now be run with the MR72. Go to the desktop and double-click on the MR72 shortcut.

